

An overview of CRISPR-artificial intelligence theranostics: Current and emerging applications

Prerna Vats^{1#}, Bhavika Baweja^{1#}, Chainsee Saini¹, Atar Singh Kushwah², Ashok Kumar³, Sandeep K. Srivastava¹, and Rajeev Nema^{1*}

ABSTRACT

Clustered regularly interspaced short palindromic repeats (CRISPR)-based diagnostics are revolutionizing precision medicine by enabling highly sensitive detection of nucleic acid and protein biomarkers. Building on these capabilities, CRISPR-based theranostics now aim to unify real-time disease detection with targeted therapeutic interventions. However, traditional CRISPR diagnostics face several limitations, including restricted multiplexing, off-target effects, and challenges in delivery efficiency. To overcome these issues, artificial intelligence (AI) has significantly enhanced CRISPR platforms by enabling intelligent guide RNA (gRNA) design, interpretation of complex biosensor outputs, and facilitation of rapid clinical decision-making. Machine learning tools such as DeepCRISPR, Azimuth 2.0, DeepHF, and CRISPRpred support the development of highly specific gRNAs, reduce off-target events, and personalize genome-editing strategies based on individual genomic profiles. Recently, by combining CRISPR systems with nanomaterials, fluorescence-based detection, and electrochemical sensing, researchers have developed advanced biosensors capable of detecting a broad spectrum of disease biomarkers, from cancer-associated nucleic acids to viral and genetic disorders. These advances support both diagnostics and gene therapy, enabling accurate, low-cost testing at home, in point-of-care settings, and in resource-limited environments. Together, the integration of AI and CRISPR is accelerating biomarker discovery and the development of intelligent, adaptive therapeutic platforms. New point-of-care diagnostic tests (POCTs) based on CRISPR-AI are essential for early screening of high-mortality diseases, and CRISPR-based diagnostic assays have emerged as powerful, versatile alternatives to traditional nucleic acid tests, offering rapid, programmable, and portable diagnostic solutions. This review explores the evolution of CRISPR-AI theranostic systems, current and emerging POCT applications. It highlights the technological, clinical, and ethical challenges shaping their translation into next-generation precision diagnostics.

Keywords:

CRISPR-Cas; Biosensing; Gene editing; Diagnostics; Precision medicine

*Authors contributed equally.

*Corresponding author:

Rajeev Nema,
rajeev.nema@jaipur.manipal.edu

How to cite this article:

Vats P, Baweja B, Saini C, et al. An overview of CRISPR-artificial intelligence theranostics: Current and emerging applications. *Biomater Transl.* 2026, 7(1), 79-120.

doi: [10.12336/bmt.25.00106](https://doi.org/10.12336/bmt.25.00106)



1. Introduction

The clustered regularly interspaced short palindromic repeats (CRISPR) and CRISPR-associated protein (CRISPR-Cas) system, a prokaryotic adaptive immune mechanism discovered in bacteria and archaea, has emerged as a powerful and programmable platform for genome manipulation.¹ Over the past two decades, its integration with advances in

molecular biology and engineering has reshaped the landscape of precision medicine, addressing persistent challenges in disease modeling, diagnostics, and therapeutics.² Characterized by its RNA-guided nuclease (NUC) activity, CRISPR enables site-specific, efficient, and cost-effective genomic manipulation.³ Recent advancements in CRISPR technology have met the World Health Organization's "REASSURED" criteria for optimal diagnostic tools, emphasizing

real-time efficiency, affordability, high sensitivity, specificity, user-friendly design, rapidity, equipment-free usability, and direct application for end users.⁴

While earlier genome-editing tools such as zinc finger NUCs and transcription activator-like effector NUCs laid the groundwork for targeted DNA modifications,⁵ their widespread use was limited by the need for labor-intensive protein engineering, relatively high costs, and variable efficiency with significant off-target risks.⁶ In contrast, CRISPR relies on a simple RNA-guided recognition (REC) mechanism, making it far more versatile, programmable, and scalable.⁷ These features, coupled with lower costs and rapid adaptability to diverse targets, have positioned CRISPR as a transformative advance over earlier NUC-based systems. Subsequently, the introduction of CRISPR-Cas9 marked a transformative milestone by simplifying the targeting mechanism through guide RNA (gRNA)-directed DNA cleavage.⁸ This leap in accessibility revolutionized modern molecular biology and was recognized with the 2020 Nobel Prize in Chemistry awarded to Charpentier and Doudna. However, Feng Zhang, a researcher at the Broad Institute of Massachusetts Institute of Technology (MIT) and Harvard, was the first to adapt and demonstrate the CRISPR-Cas9 system for genome editing in eukaryotic cells.⁹ A timeline illustrating the evolution of genome editing technologies, from early programmable NUCs to modern CRISPR-based systems, is shown in **Figure 1**.

Beyond genome editing, CRISPR systems have been rapidly adapted for molecular diagnostics owing to the collateral cleavage activity exhibited by certain effector proteins, such as Cas12 and Cas13.¹⁰ Upon target REC, these enzymes non-specifically cleave surrounding nucleic acids, a property used for signal amplification in diagnostic assays.¹¹ This mechanism underlies the design of CRISPR-based diagnostics (CRISPR-Dx) platforms such as Specific High-Sensitivity Enzymatic Reporter UNLOCKing (SHERLOCK), DNA endonuclease targeted CRISPR trans reporter (DETECTR), 1-h low-cost multipurpose highly efficient system (HOLMES), and FnCas9 editor linked uniform detection assay (FELUDA), which have demonstrated high sensitivity and specificity for detecting viral, bacterial, and cancer-associated nucleic acids. These platforms fulfill the World Health Organization's REASSURED criteria and offer decentralized, rapid, and cost-effective alternatives to conventional nucleic acid testing.¹² Furthermore, integration with nanomaterials, fluorescent reporters, and electrochemical biosensors has enabled multiplexing, improved signal transduction, and enhanced detection sensitivity.¹³ As a result, CRISPR-Dx systems are now being developed for point-of-care test (POCT) and even at-home applications, with increasing relevance in infectious disease surveillance, oncology, and resource-limited clinical settings.¹⁴

In parallel with their diagnostic applications, CRISPR technologies have diversified beyond double-stranded DNA

(dsDNA) cleavage to enable precise and programmable control over gene expression.¹⁵ Catalytically inactivated Cas9 (dCas9) fused to transcriptional repressors or activators forms the basis of CRISPR interference (CRISPRi) and CRISPR activation (CRISPRa), respectively—tools that allow programmable gene silencing or upregulation without altering the underlying genomic sequence.¹⁶ These systems have been instrumental in elucidating gene function and modeling disease phenotypes in a reversible and non-mutagenic manner.¹⁷ Further advances, such as base editors that enable single-nucleotide substitutions without double-stranded breaks (DSBs), extend precision to targeted insertions, deletions, or sequence replacements,¹⁸ thereby enhancing the safety and specificity of genome engineering while opening new avenues in synthetic biology, biosensor development, and theranostic circuit design.¹⁹ Ultimately, these advances expand the functional landscape of gene manipulation and set the stage for context-responsive therapeutic interventions.

Despite their transformative potential, CRISPR-based technologies face persistent challenges such as off-target effects, suboptimal gRNA design, and context-specific variability in editing efficiency.²⁰ To overcome these limitations, artificial intelligence (AI) and machine learning (ML) are increasingly being integrated with CRISPR systems, offering data-driven solutions for enhancing precision, scalability, and personalization.²¹ AI-based platforms such as DeepCRISPR, Azimuth 2.0, CRISPRpred, and Deep post-Hartree-Fock (DeePHF) have demonstrated high performance in predicting gRNA activity, minimizing off-target risks, and enabling rational design of genome-editing strategies across diverse biological contexts.²² These tools analyze vast genomic datasets, epigenetic landscapes, and sequence-structure features to generate optimized gRNA candidates tailored to specific cell types and disease states.²³ Furthermore, AI-driven analytics are being incorporated into biosensing platforms to automate signal interpretation, noise reduction, and threshold calibration, thus enhancing diagnostic accuracy and decision-making.²⁴ The integration of AI not only addresses the inherent complexity of biological systems but also lays the foundation for next-generation CRISPR platforms that are intelligent, adaptive, and clinically actionable. The association of CRISPR with AI, nanotechnology, and biosensor engineering is giving rise to a new generation of programmable theranostic platforms, capable of both detecting disease biomarkers and executing context-specific therapeutic interventions.²⁵ These CRISPR-AI-integrated systems are now being explored for use in POCT, offering rapid, portable, and programmable diagnostic solutions for high-mortality diseases such as cancer, infectious disorders, and genetic syndromes.²⁶ By combining AI's predictive capabilities with CRISPR's molecular precision, such platforms hold the potential to enable closed-loop therapeutic circuits that can sense, diagnose, and respond in real time.²⁷ However, the path toward clinical adoption is shaped by significant translational challenges, including delivery

¹Department of Biosciences, Manipal University Jaipur, Dehmi Kalan, Jaipur-Ajmer Expressway, Jaipur, Rajasthan, India; ²Women's Biomedical Research Institute, Icahn School of Medicine at Mount Sinai, New York, United States of America; ³Department of Biochemistry, All India Institute of Medical Sciences, Bhopal, Saket Nagar, Bhopal, Madhya Pradesh, India

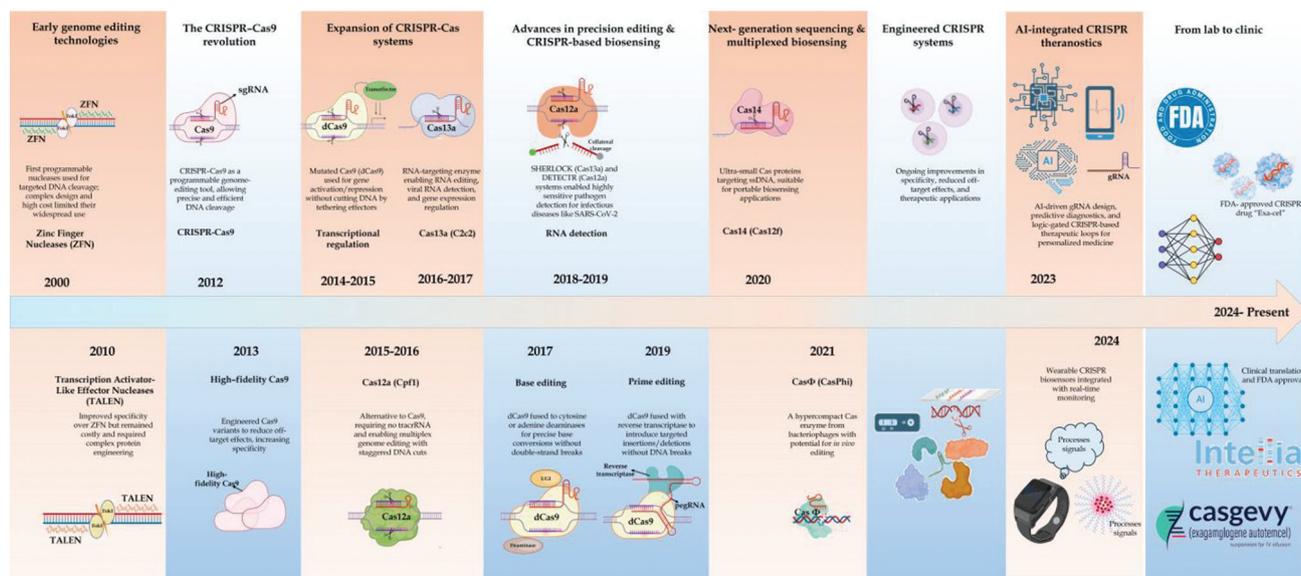


Figure 1. Timeline of genome editing technologies, highlighting significant advancements from early programmable nucleases to modern CRISPR-based systems. Figure created by the authors.

Abbreviations: AI: Artificial intelligence; Cas: CRISPR-associated protein; CRISPR: Clustered regularly interspaced short palindromic repeats; dCas: Catalytically inactivated Cas; DETECTR: DNA endonuclease targeted CRISPR trans reporter; FokI: *Flavobacterium okeanokoites* restriction endonuclease; gRNA: Guide RNA; pegRNA: Prime editing guide RNA; SHERLOCK: Specific High-sensitivity Enzymatic Reporter unLOCKing; ssDNA: Single-stranded DNA; tracrRNA: Trans-activating CRISPR RNA; UGI: Uracil-DNA glycosylase inhibitor.

efficiency, biomolecular stability, regulatory complexity, and ethical concerns surrounding genome manipulation and data use.

In this review, we present a comprehensive synthesis of current CRISPR-AI applications in diagnostics and emerging theranostic systems. We explore their underlying principles, the role of biosensors as key enabling technologies, and their real-world potential in point-of-care and personalized medicine. Furthermore, we critically examine the technical, clinical, and ethical challenges that must be addressed to ensure their successful integration into future precision medicine frameworks.

2. The CRISPR-Cas toolkit

CRISPR-Cas systems consist of several key components, including a Cas protein, CRISPR RNA (crRNA), and trans-activating CRISPR RNA (tracrRNA).²⁸ The Cas protein, such as Cas9, functions as a molecular scissor, directed by the crRNA to cleave the targeted sequence.²⁹ tracrRNA is essential for the pre-processing of precursor CRISPR RNA (pre-crRNA) into the mature functional crRNA form, facilitating the assembly of a ribonucleoprotein (RNP) complex that carries out genome targeting.³⁰ Together, these elements have enabled scientists to precisely modify the genetic code, interrogate gene functionality, develop new treatments for hereditary diseases, and create genetically modified organisms with specific traits.^{31,32} Importantly, variations in these core components have led to the development of various CRISPR systems with unique functionalities applicable to diagnostics, biosensing, and next-generation theranostics.³³ Thereby, understanding the role of each component in the CRISPR-Cas system is crucial to fully utilizing its potential in genetic engineering. A detailed summary of these components, their molecular

roles, and diverse applications is presented in **Table 1**. While the toolkit outlines the structural components of CRISPR, understanding how these parts cooperate in natural immunity provides context for their repurposing in genome editing, as described in the following section.

2.1. Core components

2.1.1. Cas proteins

CRISPR-associated proteins are the catalytic core of the CRISPR-Cas system, functioning as molecular scissors to recognize and cleave nucleic acid sequences.⁷ Cas proteins recognize specific protospacer adjacent motifs (PAM), as explained further in Section 2.1.4, enabling adaptability in targeting different genomic regions.⁴⁰ Cas9, derived from *Streptococcus pyogenes*, is the most widely used Cas variant due to its precision and ease of use in genome editing.⁴¹ Cas12 and Cas14 possess collateral cleavage activity, allowing them to degrade non-target single-stranded DNA (ssDNA) after recognizing a target, an essential property of biosensors to amplify detection signals.⁴² Cas13 specifically targets RNA, broadening the applications of CRISPR to transcriptomic regulation and RNA virus diagnostics.⁴³ The recently characterized Cas Φ , a compact NUC encoded by bacteriophages, offers high gene editing efficiency, particularly in resource-limited or viral vector-constrained environments.⁴⁴ In addition, modified Cas proteins with expanded or altered PAM specificities have increased their applicability, enabling multiplexed targeting of various genomic regions.⁴⁵ Cas proteins also serve as effectors in base editing and prime editing systems, two advanced technologies that allow precise nucleotide conversion without inducing DSBs.⁴⁶ The incorporation of Cas proteins into biosensors presents significant potential for point-of-care diagnostics, enabling swift and accurate identification

Table 1. Key components of CRISPR-Cas systems and their applications

CRISPR-Cas component	Description	Key application (s)	References
Cas protein (e.g., Cas9, Cas12, Cas13)	“Molecular scissors” that cleave nucleic acids (DNA or RNA). Different Cas proteins have distinct cleavage mechanisms and target-specific types of nucleic acids	Gene knockout, insertion, or correction via DNA/RNA cleavage	34
Guide RNA (gRNA)/ single guide RNA	A synthetic RNA molecule that directs the Cas protein to a specific target sequence in the genome. It consists of a spacer sequence (complementary to the target DNA/RNA) and a scaffold sequence (binds to the Cas protein)	Ensures site-specific cleavage	35
Protospacer adjacent motif	A short, specific DNA sequence located adjacent to the target (protospacer) sequence. Recognized by Cas proteins and essential for their binding and cleavage activity	Determines where Cas can bind and cut	36
Dead Cas (dCas) variants (e.g., dCas9, dCas12, dCas13)	Catalytically inactive Cas proteins (mutated to prevent DNA/RNA cleavage) that retain their ability to bind to specific DNA/RNA sequences when guided by gRNA	Gene regulation, imaging, epigenetic editing	37
Base editors (e.g., CBE, ABE)	Fusion proteins combining a dCas protein with a deaminase enzyme. These systems enable precise single-nucleotide changes without introducing double-strand breaks	Correct point mutations without DNA breaks	38
Prime editors	Advanced gene editing tools combining a Cas9 nickase (which cuts only one DNA strand), a reverse transcriptase, and a prime editing guide RNA	Precise insertions, deletions, or base changes	39

Abbreviations: ABE: Adenine base editor; CBE: Cytosine base editors; CRISPR-Cas: Clustered regularly interspaced short palindromic repeats and CRISPR-associated protein.

of diseases and pathogens, thereby improving personalized medicine and environmental monitoring.

2.1.2. crRNA and tracrRNA

crRNA and tracrRNA are central to the RNA-guided mechanism of most Class 2 CRISPR systems.⁴⁷ The crRNA contains a sequence complementary to the target DNA (the spacer) and a repeat-derived sequence that binds tracrRNA.⁴⁸ The tracrRNA is essential for crRNA maturation and for recruiting Cas proteins to form a functional RNP complex.⁴⁹ In native systems, the tracrRNA and crRNA operate as two distinct molecules; however, they are often fused into a single gRNA (sgRNA) in laboratory applications to streamline genome editing protocols.⁵⁰ This programmable dual-RNA complex directs the Cas protein to its target with high sequence specificity, forming the molecular basis for genome and transcriptome editing.⁵¹

2.1.3. gRNA

In most applications, crRNA and tracrRNA (discussed in Section 2.1.2) are fused into a sgRNA, simplifying design for genome editing and diagnostics. It consists of a ~20-nucleotide spacer sequence that is complementary to the target DNA or RNA, and a scaffold region that forms the necessary secondary structures for Cas binding.⁵² The gRNA-Cas complex scans the genome for PAM-adjacent regions. It induces cleavage or modulation only on successful base-pairing with the target.⁵³ Precision in gRNA design is critical for minimizing off-target activity and improving editing efficiency. AI-driven tools such as Benchling, CRISPR-DO, and sgRNA Designer are increasingly used to predict gRNA activity and specificity, optimizing their application in both therapeutic and diagnostic platforms, as listed in **Table 2**.⁵⁴

2.1.4. PAM

The PAM is a short, conserved DNA sequence flanking the target site that is essential for Cas protein binding and initiation of the editing process.⁸¹ The PAM sequence varies across Cas proteins, such that Cas9 recognizes NGG, whereas Cas12a recognizes TTTV. PAMs play a vital role in distinguishing self from

non-self DNA, thereby preventing autoimmune targeting of the host genome.⁴⁶ Identifying and utilizing the appropriate PAM sequences can significantly enhance the efficiency and accuracy of CRISPR-based genome editing. In biosensing, PAM-dependent activation of Cas12 ensures signal specificity, which increases the potential for multiplexed detection of nucleic acid biomarkers in CRISPR-Dx platforms.⁴² Despite their essential role, PAM requirements can also restrict CRISPR applications by limiting the number of accessible genomic sites, particularly in AT- or GC-rich regions.⁸² To overcome this bottleneck, researchers have engineered Cas variants with relaxed or altered PAM REC, such as SpRY, SpCas9-NG, and evolved Cas12a proteins, which expand the range of editable targets.⁸³ In addition, PAM-independent approaches such as base editors, prime editors, and CRISPR-associated transposases bypass conventional PAM constraints, thereby broadening the versatility of CRISPR-based genome engineering.⁸⁴ These innovations collectively enhance the flexibility, precision, and translational applicability of CRISPR systems across diverse biological contexts.

Taken together, these components not only operate in coordination but also differ in ways that define their application potential. For example, Cas9 remains the standard for dsDNA cleavage, whereas Cas12 extends functionality through collateral ssDNA cleavage for diagnostic assays, and Cas13 uniquely targets RNA, enabling transcriptome editing and RNA virus detection.⁸⁵ Similarly, while natural systems rely on separate crRNA and tracrRNA molecules, the laboratory-engineered sgRNA simplifies experimental workflows by merging these roles into a single guide molecule. PAM further distinguishes Cas9 and Cas12 systems by constraining targetable loci, in contrast to Cas13, which does not require PAM sequences.⁸⁶ These distinctions shape the choice of effector systems for specific tasks such as genome engineering, transcriptome regulation, or rapid biosensing, highlighting the adaptability of the CRISPR toolkit.

2.2. CRISPR array

The CRISPR array is a locus within the microbial genome consisting of short, repetitive DNA sequences interspersed

Table 2. Tools for CRISPR guide RNA design and editing

Resource	Supported genomes	CRISPRi/a functionality	Enzymes	Link and references
Benchling	Many	No	SpCas9, SaCas9, NmeCas9, StCas9, TdCas9, Cas12a	https://www.benchling.com ⁵⁵
CHOPCHOP	Many	Yes	Cas9 (custom PAM), Cas12a, CasX, Cas13	https://chopchop.cbu.uib.no ⁵⁶
CRISPick	Human, mouse, rat	Yes	SpCas9, SaCas9, AsCas12a, enAsCas12a	https://portals.broadinstitute.org/gpp/public/analysis-tools/sgrna-design ⁵⁷
CRISPOR	Many	No	Cas9 (various PAMs), CasX, Cas12a	http://crispor.tefor.net ⁵⁸
E-CRISP	Many	Yes	SpCas9	http://www.e-crisp.org/E-CRISP ⁵⁹
FlashFry	Any reference genome	No	SpCas9, Cas12a	https://github.com/mckennalab/FlashFry ⁶⁰
GUIDES	Human, mouse	No	SpCas9	https://guides.sanjanalab.org ⁶¹
GuideScan	Human, mouse, <i>Drosophila</i> , yeast, zebrafish, <i>Caenorhabditis elegans</i>	No	SpCas9, AsCas12a	http://www.guidescan.com ⁶²
RGEN Cas-Designer	Many	No	SpCas9 (variants), SaCas9, Cas12a, Cas12b	http://www.rgenome.net/cas-designer ⁶³
Vienna Bioactivity CRISPR (VBC) score	Human, mouse, <i>Drosophila</i> , <i>C. elegans</i> , rat, <i>Xenopus tropicalis</i>	No	SpCas9	https://viennabioactivity.org ⁶⁴
Cas13design	Human, mouse, zebrafish, <i>Drosophila</i> , <i>C. elegans</i> , <i>Arabidopsis</i> , RNA viruses	NA	RfxCas13d	https://cas13design.nygenome.org ⁶⁵
BE-Hive	Human, mouse, zebrafish, <i>Drosophila</i> , <i>C. elegans</i> , <i>Arabidopsis</i> , RNA viruses	NA	CBE, ABE base editors	https://behive.broadinstitute.org ⁶⁶
DeepCRISPR	Human	No	SpCas9	https://github.com/biomedBit/DeepCRISPR ⁶⁷
PAVOOC	Human	Yes	SpCas9	https://pavooc.shinyapps.io/pavooc/ ⁶⁸
CRISPRitz	Custom genomes	No	Cas9, Cas12a, Cas13	https://github.com/pinellolab/CRISPRitz ⁶⁹
Cas-OFFinder	Custom genomes (via local install)	No	Any Cas	http://www.rgenome.net/cas-offinder ⁷⁰
CCTop	Human, mouse, zebrafish, and others	No	Cas9	https://cctop.cos.uni-heidelberg.de : 8043 ⁷¹
CRISPR-DO	Human, mouse	No	SpCas9	http://cistrome.org/CRISPR-DO ⁷²
sgRNA Scorer	Human, mouse	No	SpCas9	https://crispr.med.harvard.edu/sgRNAScorer ⁷³
CRISPRater	Human	No	SpCas9	https://sourceforge.net/projects/crisprater ⁷⁴
Cas-Designer 2.0	Human, mouse, plant genomes	No	Cas9, Cas12a, variants	https://www.rgenome.net/cas-designer-2 ⁷⁰
Deskgen	Human, mouse, custom	No	SpCas9, SaCas9, Cas12a	https://www.deskgen.com ⁷⁵
Geneious	Custom	No	SpCas9	https://www.geneious.com ⁷⁶
Horizon Discovery	Human, mouse	No	SpCas9	https://horizondiscovery.com ⁷⁷
IDT	Human, mouse, zebrafish, others	Yes	SpCas9, Cas12a	https://www.idtdna.com/pages/tools ⁷⁷
Off-Spotter	Human (custom genomes)	No	SpCas9	http://cm.jefferson.edu/Off-Spotter ⁷⁸
Synthego	Human, mouse	Yes	SpCas9	https://www.synthego.com ⁷⁹
TrueDesign	Human	Yes	SpCas9, Cas12a	https://www.thermofisher.com/truedesign ⁸⁰

Abbreviations: ABE: Adenine base editor; AsCas12a: *Acidaminococcus* sp.-derived Cas12a nuclease; Cas: CRISPR-associated protein; CBE: Cytosine base editors; CRISPRa: CRISPR activation; CRISPRi: CRISPR interference; CRISPR: Clustered regularly interspaced short palindromic repeats; enAsCas12a: Enhanced AsCas12a; NA: Not available; NmeCas9: *Neisseria meningitidis* Cas9; PAM: Protospacer adjacent motif; SaCas9: *Staphylococcus aureus* Cas9; SpCas9: *Streptococcus pyogenes* Cas9; StCas9: *Streptococcus thermophilus* CRISPR3-Cas; TdCas9: *Treponema denticola* Cas9 endonuclease deficient Cas9.

with unique spacer sequences derived from previously encountered genetic elements, such as viruses or plasmids. This array acts as a genetic memory system, enabling the CRISPR-Cas machinery to recognize and respond to recurring foreign sequences.⁸⁷ Understanding the interactions between the CRISPR array, Cas proteins, and gRNA helps scientists optimize the system for various

applications in genetic engineering. Recent advances in CRISPR technology have led to the development of more precise gene-editing tools, such as CRISPR-Cas9, which offer enhanced specificity and reduced off-target effects.⁸⁸ In addition, researchers have developed new variants, such as CRISPR-Cas12 and CRISPR-Cas13, which expand the range of applications by targeting RNA sequences, and

these innovations hold promise for the treatment of genetic disorders.⁸⁹

2.2.1. Spacer sequences

Spacer sequences are short DNA segments within the CRISPR array, derived from foreign genetic material encountered during previous infections, and serve as a molecular memory of past attacks.⁹⁰ Following the transcription of these spacer sequences into gRNA, the Cas protein is directed to the target DNA for precise editing.⁹¹ The gRNA provides the necessary instructions for the Cas protein to identify and bind to the target DNA sequence.⁴⁶ This molecular memory enables sequence-specific targeting and high-fidelity editing or interference.⁹² This specificity enables researchers to make targeted modifications without affecting other parts of the genome, making spacer sequences crucial for CRISPR-Dx platforms.

2.2.2. Repeat sequences

Repeat sequences are highly conserved, palindromic DNA elements that flank each spacer within the CRISPR array and are essential for the system's proper functioning, as they serve as REC sites for the Cas protein.²⁸ During crRNA processing, the repeats facilitate the correct folding and cleavage of the long precursor transcript into individual guide units.⁹³ By understanding the interplay between spacer and repeat sequences, further optimization of artificial CRISPR systems can be achieved for a broad set of applications, ranging from gene therapy to biotechnology.

2.3. Classification of CRISPR-Cas systems

The classical classification of CRISPR-Cas proteins was originally based on factors such as evolutionary origin, structural composition, cleavage domains, and nucleic acid targets.⁹⁴ However, with growing structural and functional insights, these systems are now broadly categorized into two major subclasses: Class 1 and Class 2, each exhibiting distinct characteristics and functions, as illustrated in **Table 3**. Class 1 systems are characterized by multi-protein effector complexes and can target a broad range of DNA sequences. This adaptability makes them vital tools for genome editing, RNA interference, and microbial defense applications.⁹⁵ In contrast, Class 2 systems are generally defined by their simplicity, comprising a single large effector protein, with CRISPR-Cas9 being the most prominent example.⁹⁶ The simplicity, efficiency, and precision of Cas9 establish it as the predominant tool in gene editing. Within these two main categories, further subdivisions are defined based on functional features and molecular components: Type I, Type III, and Type IV in Class 1, and Type II, Type V, and Type VI in Class 2.⁹⁷ Each subtype exhibits variations in components, mechanisms of interference, and target specificity, offering a diverse array of tools for genome manipulation. Type II systems (e.g., Cas9) are well-recognized for their ability to introduce DSBs, whereas Type V (e.g., Cas12) systems possess collateral cleavage activity and target DNA with high precision.^{50,98} Type VI systems, represented by Cas13, primarily function in RNA targeting, facilitating transcriptome modulations.⁹⁹ Notably, Cas14 (also termed Cas12f), classified under Type V,

Table 3. Classification of CRISPR-Cas immune systems

Class	Type	Key effector protein (s)	Target nucleic acid	Key characteristics	Common subtypes/notes (examples)
Class 1	Multi-component effector complexes				
	Type I	Cas3 (helicase/nuclease), cascade complex (CasA-E, Cas5-8)	DNA	Most abundant; Cas3 unwinds and cleaves DNA. Requires a protospacer adjacent motif (PAM)	I-A, I-B, I-C, I-D, I-E, I-F
	Type III	Cas10 (cyclase/nuclease), Csm/Cmr complex	DNA and/or RNA	Can target both DNA and RNA. Exhibits unique "collateral" RNA cleavage activity upon target binding	III-A, III-B, III-C, III-D, III-E, III-F
Type IV	Cas5, Cas7, Csf1 (small Cas8-like)	DNA (likely)	Less understood; often plasmid-encoded. Lacks Cas1/Cas2 for adaptation. Simpler architecture	IV-A, IV-B, IV-C	
Class 2	Single-component effector proteins				
	Type II	Cas9	DNA	Widely used for genome editing; single effector protein. Requires crRNA and tracrRNA (often fused as sgRNA). PAM-dependent	II-A (SpCas9), II-B (Cas4-containing), II-C (minimal systems like FnCas9)
	Type V	Cas12 (e.g., Cas12a/Cpf1, Cas12b, Cas12c, Cas12d, Cas12e, Cas12f, Cas12g, Cas12h, Cas12i, Cas12u)	DNA	Creates staggered DNA cuts; diverse PAM requirements; exhibits collateral ssDNA cleavage	V-A (Cas12a/Cpf1), V-B (Cas12b/C2c1), V-C (Cas12c/C2c3), V-D (Cas12d/CasY), V-E (Cas12e/CasX), V-F (Cas12f/CasRx), V-G, V-H, V-I, V-U
	Type VI	Cas13 (e.g., Cas13a/C2c2, Cas13b, Cas13c, Cas13d)	RNA	Exclusively targets RNA. Possesses collateral RNA cleavage activity	VI-A (Cas13a), VI-B (Cas13b), VI-C (Cas13c), VI-D (Cas13d/CasRx)
	New discoveries	SubCas9 (from <i>Streptococcus uberis</i>)	DNA	Smaller than traditional Cas9; potentially less immunogenic. Targets different genetic sequences	Yet to be fully classified; candidate for inclusion in Type II

Abbreviations: Cas: CRISPR-associated protein; CRISPR-Cas: Clustered regularly interspaced short palindromic repeats and CRISPR-associated protein; crRNA: CRISPR RNA; Csm: Type III-A complexes; Cmr: Type III-B complexes; sgRNA: Single guide RNA; tracrRNA: Trans-activating CRISPR RNA.

has emerged as a hypercompact effector with high specificity for ssDNA, expanding the CRISPR toolkit for applications requiring minimal off-target activity and compatibility.¹⁰⁰ Current CRISPR research continues to focus on refining the classification of interference mechanisms, as advancements in these areas can significantly enhance the specificity and efficiency of gene-editing technologies. While this section has outlined the core components of the CRISPR toolkit, the following section (Section 3) focuses on how these components operate together through the processes of adaptation, expression, and interference.

3. Mechanism of the CRISPR-Cas system

Building on the description of individual components in Section 2, this section discusses the coordinated mechanisms—adaptation, expression, and interference—through which the CRISPR-Cas system functions. These stages collectively enable prokaryotes to recognize and neutralize foreign genetic elements and serve as the foundation for the system's adaptation in gene editing, diagnostics, and biosensing.¹⁰¹⁻¹⁰³ Furthermore, this system relies on essential defense mechanisms, including transcription, crRNA biogenesis, and target degradation.⁹⁴ The mechanism is illustrated in **Figure 2** and described in detail in **Table 4**.

3.1. Adaptation

The adaptation phase initiates the CRISPR-Cas immune response by facilitating the acquisition and genomic integration of foreign DNA fragments, termed protospacers, derived

from invading mobile genetic elements such as plasmids or bacteriophages.¹⁰⁴ These protospacers are inserted into the CRISPR array as new spacer sequences, flanked by conserved repeat elements. The integration process is carried out by the Cas1-Cas2 protein complex, which selectively captures foreign DNA and inserts it near the leader sequence of the CRISPR array.¹⁰⁷ These spacers function as genetic repositories, allowing the system to identify and target exogenous DNA during subsequent infections.¹⁰⁸ In engineered systems, the principle of spacer acquisition has inspired the design of synthetic gRNAs to direct Cas proteins to specific genomic loci for targeted editing.¹⁰⁹ The ability to define multiple spacers in CRISPR arrays has enabled multiplexed gene editing, allowing for the simultaneous modification of several genes in a single experiment.¹¹⁰ Moreover, this programmable specificity is fundamental to the creation of sensitive and programmable biosensors, providing high sensitivity, cost-effectiveness, and rapid detection of genetic material, essential for point-of-care diagnostics and real-time mutation tracking.⁹⁸ In addition, the adaptation phase is crucial for the long-term evolution of bacterial immunity, as it enables the system to respond to evolving genetic threats.¹¹¹ Collectively, this phase ensures both the adaptability of CRISPR-Cas systems in nature and their flexibility as tools in synthetic biology, diagnostics, and precision therapeutics.

3.2. Expression

The expression phase involves transcribing the CRISPR array into a long pre-crRNA, containing alternating repeat

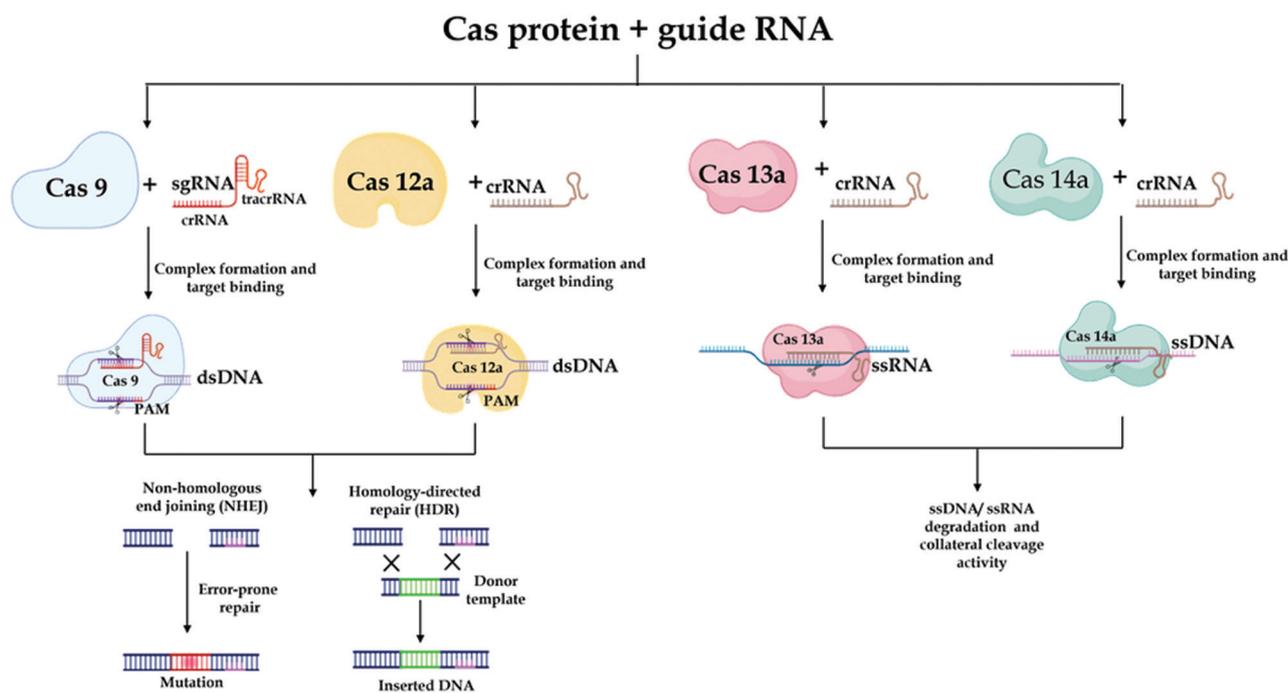


Figure 2. Comparative mechanisms of different Cas proteins in genome and transcriptome editing. Cas9 and Cas12a target dsDNA, inducing double-strand breaks that are repaired via non-homologous end joining or homology-directed repair. Cas13a targets ssRNA, leading to its degradation and collateral RNA cleavage. Cas14a targets ssDNA with collateral cleavage activity, making it useful for biosensing applications. Figure created by the authors.

Abbreviations: Cas: CRISPR-associated protein; crRNA: CRISPR RNA; dsDNA: Double-stranded DNA; PAM: Protospacer adjacent motif; sgRNA: Single guide RNA; ssRNA: Single-stranded RNA; ssDNA: Single-stranded DNA; tracrRNA: Trans-activating CRISPR RNA.

Table 4. Molecular mechanism of CRISPR-Cas system: Three main stages

Stage	Description	Key molecular players and steps	Outcome/function	References
1. Adaptation (spacer acquisition)	The prokaryotic cell “remembers” a foreign invader by acquiring a small piece of its DNA and integrating it into its own genome. This creates a genetic “memory of past infections	(i) Recognition of foreign DNA: When a phage or plasmid invades, specific Cas proteins (primarily Cas1 and Cas2) identify and capture a short segment of the foreign DNA, known as a “protospacer.” This process is often influenced by sequence motifs on the foreign DNA (ii) Integration into CRISPR array: The protospacer is then inserted as a new “spacer” into the CRISPR locus of the host genome. New spacers are typically added at one end of the CRISPR array, creating a chronological record of infections. This integration is accompanied by the duplication of an adjacent “repeat” sequence	Genetic memory: The host genome gains a new, unique spacer sequence, effectively “immunizing” the cell against future attacks by the same or similar invaders	104-106
2. Expression (crRNA biogenesis/maturation)	The integrated genetic memory (CRISPR array) is transcribed and processed into small functional RNA molecules that will guide the Cas proteins	(i) Transcription of CRISPR array: The entire CRISPR locus (repeats and spacers) is transcribed into a long precursor CRISPR RNA (pre-crRNA) (ii) Processing of pre-crRNA: This transcript is cleaved by specific Cas ribonucleases (e.g., Cas6 in some systems or Cas9 aided by tracrRNA in Type II systems) into individual mature CRISPR RNAs (crRNAs), each containing a single spacer sequence flanked by partial repeat sequences (iii) Assembly of effector complex: The mature crRNAs associate with one or more Cas proteins to form a functional ribonucleoprotein (RNP) complex, also called a surveillance complex (e.g., cascade in Type I, or Cas9 alone in Type II)	Formation of guided surveillance complexes: Ready-to-use “search-and-destroy” complexes are formed, pre-programmed with genetic information from past invaders	
3. Interference (targeting)	Upon reinvasion by the same foreign nucleic acid, the pre-programmed Cas-crRNA complex recognizes and degrades the invader. This is the “active defense” phase	(i) Target scanning and recognition: The Cas-crRNA complex continuously scans the cell for foreign nucleic acids that match its spacer sequence. Recognition also requires the presence of a protospacer adjacent motif (PAM) sequence (in DNA-targeting systems) for efficient binding (ii) Base pairing: If a match is found and the PAM is present, the crRNA base-pairs with the complementary sequence on the foreign DNA or RNA (iii) Cleavage of target: The Cas protein’s nuclease domain is activated, leading to the precise cleavage and degradation of the invading nucleic acid, thereby neutralizing the threat	Immunity and invader elimination: The foreign genetic material is destroyed, preventing successful infection or replication by the pathogen or plasmid	

Abbreviations: CRISPR-Cas: Clustered regularly interspaced short palindromic repeats and CRISPR-associated protein; pre-crRNA: Precursor CRISPR RNA; tracrRNA: Trans-activating CRISPR RNA.

and spacer sequences.¹¹² This precursor is subsequently processed into individual crRNAs, each encoding the sequence information of a single spacer corresponding to a previously acquired protospacer.¹²¹ In many systems, this processing requires a tracrRNA, which hybridizes to the repeat region and recruits RNase III to cleave the pre-crRNA. The resulting mature crRNAs associate with Cas proteins to form an active RNP complex capable of recognizing target nucleic acids.¹²² To streamline the system for biotechnological and therapeutic applications, many platforms use synthetic gRNAs, which are crucial for directing Cas proteins to specific DNA or RNA sequences.⁴⁶ This process significantly improves the specificity and efficiency of genome editing, enabling targeted knockouts, insertions, and gene corrections through homology-directed repair (HDR) or base editing.¹¹⁵ Well-designed gRNAs help reduce off-target effects, which is crucial for therapeutic applications. In recent years, an expanding ecosystem of computational and AI-driven platforms has leveraged the expression and modification of gRNAs to control gene expression, build genetic circuits, and reprogram cells, supporting precise genetic alterations with controlled timing and frequency.¹¹⁶ These tools analyze factors such as sequence context, secondary structure, chromatin accessibility, and mismatch tolerances to predict gRNA activity.

3.3. Interference

The interference phase is the effector stage of the CRISPR-Cas immune system, during which the CRISPR-derived RNA guides the Cas protein to locate and neutralize target nucleic acids.¹¹⁷ Following the expression and processing of gRNAs, the mature crRNA (or engineered sgRNA) forms an RNP complex with a Cas effector, enabling site-specific surveillance of invading DNA or RNA.¹¹⁸ The REC process depends on the sequence complementarity between the gRNA and the protospacer region of the target, typically adjacent to a PAM in DNA-targeting systems.¹¹⁹ Upon binding, the CRISPR-Cas complex undergoes structural activation and initiates site-specific cleavage of the target nucleic acid. This molecular interference is central not only to natural immunity but also to the programmable functions of CRISPR in synthetic applications.¹²⁰ In DNA-targeting systems, interference involves double-stranded cleavage mediated by conserved NUC domains, while RNA-targeting systems use RNA-guided cleavage without the requirement for PAM REC.¹²¹ Some systems also exhibit collateral cleavage activity, wherein non-target ssDNA or single-stranded RNA (ssRNA) molecules are degraded on activation.¹²² This property has been repurposed in CRISPR-Dx to amplify detection signals

in real-time biosensing assays. Through this programmable interference process, CRISPR-Cas systems have emerged as precision genome engineering tools, unlocking a wide range of possibilities in research, medicine, and biotechnology.¹⁶

3.3.1. REC of target DNA sequences

Target REC is a critical step in CRISPR-Cas interference, during which the gRNA-Cas complex locates a specific nucleic acid sequence based on base-pair complementarity.⁷ In DNA-targeting systems, REC typically begins with the identification of a PAM, which signals the Cas effector to initiate local DNA unwinding.¹²³ The gRNA then probes for sequence complementarity, leading to the formation of an R-loop structure if a match is found. This interaction ensures specificity and triggers the downstream cleavage mechanism.¹²⁴ In RNA-targeting systems, where PAM REC is not required, target REC is driven solely by sequence pairing and target accessibility.¹²⁵ The precision of this step is essential for both genome editing fidelity and the sensitivity of CRISPR-Dx.

3.3.2 Binding and cleavage by Cas Protein

Once the gRNA-Cas complex has successfully recognized its target, stable binding induces a conformational change in the Cas protein, activating its endonuclease activity.¹²⁶ This activation leads to the site-specific cleavage of the target nucleic acid. In DNA-targeting systems, both strands of the DNA are typically cleaved, while RNA-targeting systems cleave ssRNA targets.^{127,128} The precision of cleavage depends on stable guide-target pairing and proper alignment of the catalytic site with the cleavage region. This tightly regulated process forms the basis for programmable gene editing, allowing for the insertion, deletion, or replacement of genetic material with high specificity. In diagnostic platforms, cleavage activity is often coupled with signal amplification to enable sensitive and rapid detection.¹²⁹

3.3.3 Mechanisms of repair and gene editing

Following DNA cleavage by the CRISPR-Cas complex, the host cell activates endogenous DNA repair pathways to resolve the break. The two major mechanisms are non-homologous end joining (NHEJ) and HDR.¹³⁰ NHEJ directly ligates the broken DNA ends and often introduces insertions or deletions (indels), resulting in gene disruption. In contrast, HDR utilizes a homologous DNA template to precisely insert or correct genetic sequences at the cleavage site.¹³¹ The balance between these pathways determines the outcome of gene editing and is influenced by cell type, cell cycle stage, and template availability. Harnessing these repair mechanisms allows CRISPR to be used for both gene knockouts and precise genomic modifications.

3.3.4. CRISPRa/CRISPRi regulation

Beyond genome editing, catalytically inactive variants of Cas proteins have enabled transcriptional regulation through CRISPRi and CRISPRa.¹³² In CRISPRi, a deactivated Cas protein (dCas) is guided to a gene promoter or coding region to sterically block transcription, effectively silencing gene expression.¹³³ Conversely, CRISPRa employs dCas fused to transcriptional activators to enhance gene expression without

altering the underlying DNA sequence.¹³⁴ These systems offer precise, reversible, and multiplexed control of gene networks, allowing researchers to interrogate gene function and disease pathways without introducing permanent genetic alterations. As a result, CRISPRa/i approaches are widely used in functional genomics, cell reprogramming, and therapeutic gene modulation.¹³⁵

4. Diagnostic utility of CRISPR effectors

CRISPR-Cas systems have emerged as powerful tools not only for genome editing but also for next-generation molecular diagnostics. The programmable nature of Cas effectors, combined with their high specificity and sensitivity, has enabled the development of novel detection platforms capable of identifying nucleic acid targets with remarkable precision, as outlined in **Table 5**.¹³⁶ Unlike traditional diagnostics that rely on extensive thermal cycling or probe hybridization, CRISPR-based assays can operate under isothermal conditions and exploit the unique cleavage activities of Cas proteins to generate easily detectable signals.¹³⁷ These features make them ideal candidates for POCT and portable diagnostics, especially in resource-limited settings. This section explores the diagnostic applications of key CRISPR effectors such as Cas9, Cas12, Cas13, and Cas14, focusing on their underlying mechanisms, molecular properties, and real-world implementations in nucleic acid detection platforms. Beyond genome manipulation, the unique collateral activities of Cas proteins have rapidly expanded their use into molecular diagnostics and biosensing, as discussed below.

4.1. Cas9

The CRISPR-Cas9 system is the most widely characterized Class 2 CRISPR effector and remains the cornerstone of CRISPR-Dx. Cas9 is a dual-lobed endonuclease composed of a REC lobe and a NUC lobe, which consists of the RuvC and HNH domains responsible for cleaving the non-complementary and complementary DNA strands, respectively.¹⁶⁰ Furthermore, the target engagement requires a 5'-NGG-3' PAM, following which an sgRNA directs Cas9 to form an RNA-DNA hybrid (R-loop) and initiates site-specific DSBs.¹⁶¹ Hence, this molecular specificity enables its application in diagnostics, where both catalytically active Cas9 and its NUC-deactivated variant (dCas9) are repurposed for nucleic acid sensing.¹⁶² In addition, in cleavage-based formats, Cas9 generates specific DSBs following amplification of the target sequence, releasing detectable reporters through fluorescent or lateral flow readouts. For example, Zhu *et al.*¹⁶³ developed a Cas9-based lateral flow biosensor capable of detecting *Mycoplasma pneumoniae* with a sensitivity of three copies and 100% accuracy in 123 clinical samples within 30 min.

In contrast, dCas9 enables non-cleaving, binding-based platforms such as CRISPR/dCas9-mediated enzyme-linked immunosorbent assay (ELISA) or Bio-SCAN, where sequence-specific DNA REC is coupled with optical or electrochemical signal generation.^{164,165} **Figure 3** illustrates two such diagnostic formats: a dCas9-mediated ELISA and a Cas9-mediated lateral flow assay. These platforms are adaptable across targets ranging

Table 5. Commercially available CRISPR-Cas-based diagnostic kits

Nuclease	Technique	Preamplification	Detection method	Targeted pathogens/ organisms	LOD (copies per mL)	References
Cas9a	NASBACC	NASBA	Electronic optical reader	Zika/dengue	6.0×10 ⁵	138
	CRISDA	PCR	Fluorescence spectrophotometer	SNPs	1.5×10 ²	139
	CAS- EXPAR	EXPAR	Real-time fluorescence monitoring	Sensing of methylated DNA; <i>Listeria monocytogenes</i> mRNA	4.9×10 ²	140
	CASLFA	PCR	Paper-based LF device	African swine fever virus	20 copies/reaction	141
	FELUDA	RPA/PCR	Paper-based LF device	SARS-CoV-2 virus	10 ⁴	142
	CRISPR- chip	-	Electrochemical	gDNA from cell lines and DMD patients	1.4 x 10 ⁵	143
	FLASH	PCR	NGS	Antimicrobial resistance	1.1×10 ³	144
	Cas9nAR	Strand- displacing DNA polymerase	Fluorescence	<i>Escherichia coli</i> , <i>Saccharopolyspora erythraea</i> ; KRAS SNPs in cell lines	1.0×10 ²	145
Cas12a	DETECTR	LAMP	Paper-based LF device	HPV16/18	6.0×10 ²	146
	HOLMES	PCR	Fluorescence spectrophotometer	Japanese encephalitis virus, pseudorabies virus	6.6×10 ³	147
	E-CRISPR	-	Electrochemical	DNA: HPV16, parvovirus B19; protein: TGFβ1	3.0×10 ¹⁰	148
	CRISPR- MTB	RPA	Fluorescence or μPAD	<i>Mycobacterium tuberculosis</i>	1–100 copies/ reaction	149
Cas12b	CDetection	RPA	Fluorescence	HPV, ABO blood genotyping, BRCA1, and TP53 SNPs	6.0×10 ²	150
	HOLMES v2	LAMP	Fluorescence	RNA virus, human mRNA, circRNA, and DNA methylation	6.0×10 ³	151
	STOPCovid	LAMP	Fluorescence, LF device	SARS-CoV-2	2.0×10 ³	386
Cas12f (Cas14)	Cas14-DETECTR	PCR	Fluorescence	HERC2 SNPs in human samples	6.0×10 ³	152
Cas13a	SHERLOCK	NASBA or RPA	Fluorescence spectrophotometer/ Paper-based LF device	Virus/bacteria/cancer mutation	1.2×10 ³	153
	SHERLOCKv2	RPA	LF device	Virus/bacteria/cancer mutation	4.8	154
	CREST	RPA/PCR	Fluorescence spectrophotometer/ Paper-based LF device	SARS-CoV-2	100 copies/μL	155
	CARMEN	PCR	Fluorescence spectrophotometer	HIV, influenza A strains	5.4×10 ²	156
	CARVER	PCR	Fluorescence spectrophotometer	Viral RNA	500 attomole (~3.01×10 ⁵ copies/mL)	157
	SHINE	RPA	Fluorescence or lateral flow	SARS-CoV-2	5.0×10 ³	158
	APC- Cas	DNA polymerase	Fluorescence	<i>Salmonella enteritidis</i>	-	140
	PECL- CRISPR	EXPAR	Electrochemiluminescence	miRNA	6.0×10 ⁵	159

Abbreviations: APC-Cas: Allosteric Probe-Initiated Catalysis and CRISPR-Cas13a system; BRCA1: BReast CAncer gene 1; CARMEN: Combinatorial arrayed reactions for multiplexed evaluation of nucleic acids; CARVER: Cas13-assisted restriction of viral expression and readout; CASLFA: Cas9-mediated lateral flow nucleic acids assay; CAS-EXPAR: CRISPR/Cas9-triggered isothermal exponential amplification reaction; CDetection: Cas12b-mediated DNA detection; circRNA: Circular RNA; CREST: Cas13-based, rugged, equitable, scalable testing; CRISDA: CRISPR-Cas9-triggered nicking endonuclease-mediated strand displacement amplification method; CRISPR-Cas: Clustered regularly interspaced short palindromic repeats and CRISPR-associated protein; DETECTR: DNA endonuclease targeted CRISPR trans reporter; DMD: Duchenne muscular dystrophy; EXPAR: Exponential amplification reaction; E-CRISPR: CRISPR-Cas12a (cpf1)-based electrochemical biosensor; FELUDA: FnCas9 editor linked uniform detection assay; FLASH: Finding low abundance sequences by hybridization; gDNA: Genomic DNA; HERC2: Giant E3 ubiquitin protein ligase; HOLMES: One-hour low-cost multipurpose highly efficient system; HPV: Human papillomavirus; KRAS: Kirsten rat sarcoma virus; LAMP: Loop-mediated isothermal amplification; LF: Lateral flow; LOD: Limit of detection; mRNA: Messenger RNA; miRNA: MicroRNA; MTB: *Mycobacterium tuberculosis*; NASBA: Nucleic acid sequence-based amplification; NASBACC: Nucleic acid sequence-based amplification-CRISPR cleavage; PCR: Polymerase chain reaction; PECL-CRISPR: CRISPR/Cas13a powered portable emitter coupled logic chip; RPA: Recombinase polymerase amplification; SHERLOCK: Specific High-sensitivity Enzymatic Reporter unLOCKing; SHINE: Streamlined Highlighting of Infections to Navigate Epidemics; SNPs: Single nucleotide polymorphisms; STOP: SHERLOCK testing in one pot; TGFβ1: Transforming growth factor beta 1; TP53: Tumor protein p53.

from SARS-CoV-2 and foodborne pathogens to antimicrobial resistance genes, highlighting Cas9's diagnostic versatility.¹⁶⁶⁻¹⁶⁸ Notably, to address PAM constraints and off-target concerns, engineered variants such as *Francisella novicida*-derived

Cas9 (FnCas9) and high-fidelity variant of *S. pyogenes* Cas9 (SpCas9-HF1) have been developed with relaxed PAM compatibility and enhanced mismatch discrimination, improving sensitivity for single-nucleotide polymorphism

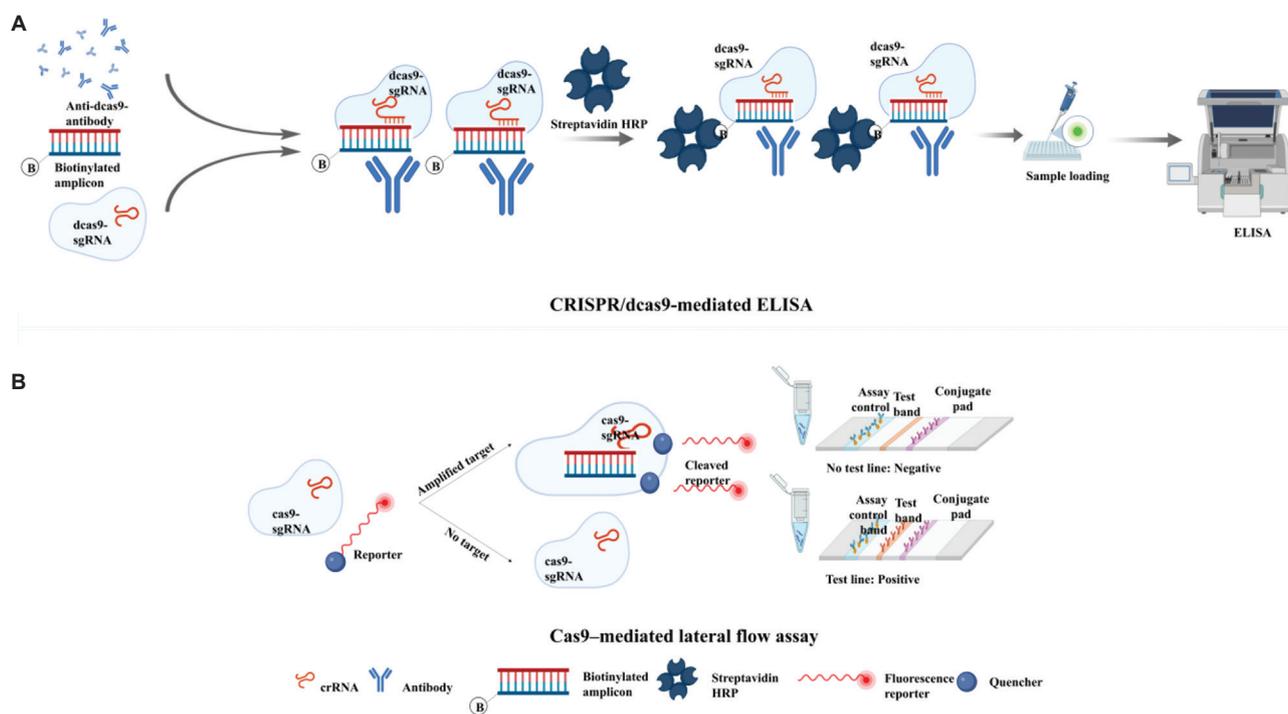


Figure 3. CRISPR-based nucleic acid detection methods: (A) dCas9-mediated ELISA and (B) Cas9-mediated lateral flow assay. In the dCas9-mediated ELISA, the dCas9–sgRNA complex binds specifically to a biotinylated target amplicon, which is captured by anti-dCas9 antibodies immobilized on a plate. Signal amplification occurs through streptavidin–HRP binding to biotin, producing a colorimetric readout upon substrate addition, which is measured using an ELISA plate reader. This method provides high specificity by leveraging the CRISPR–dCas9 system for target recognition and enzyme-linked detection for signal enhancement. In contrast, the Cas9-mediated lateral flow assay utilizes an active Cas9–sgRNA complex to detect and cleave a fluorescently labeled reporter upon target recognition. If the target is present, the reporter is cleaved, allowing detection at the test line, indicating a positive result. In the absence of the target, the uncleaved reporter flows past the test line, resulting in a negative outcome. The bottom legend defines the key molecular components involved, including crRNA, antibodies, biotinylated amplicons, streptavidin–HRP, fluorescent reporters, and quenchers. By combining the specificity of CRISPR-based detection with enzyme-linked and lateral flow-based readouts, these methods offer robust and versatile diagnostic tools for nucleic acid detection. Figure created by the authors. Abbreviations: Cas: CRISPR-associated protein; CRISPR: Clustered regularly interspaced short palindromic repeats; crRNA: CRISPR RNA; dCas9: Catalytically inactivated Cas9; ELISA: Enzyme-linked immunosorbent assay; HRP: Horseradish peroxidase; sgRNA: Single guide RNA.

detection and rare variant screening.^{169,170} Recent diagnostic studies have applied FnCas9 in lateral flow and fluorescent biosensors with attomolar sensitivity, demonstrating strong potential for clinical translation.^{171,172} Importantly, Cas9's modular architecture allows rapid reprogramming of sgRNAs, making it highly suitable for multiplexed detection and point-of-care formats.¹⁷³ These properties, along with their compatibility with low-cost amplification systems such as nucleic acid sequence-based amplification (NASBA), polymerase chain reaction (PCR), strand displacement amplification (SDA), and finding low-abundance sequences by hybridization, have led to their incorporation in emerging diagnostic workflows for infectious diseases, cancer mutation profiling, and even food safety monitoring.^{174,175} Together, the mechanistic precision, engineering flexibility, and real-world clinical performance of Cas9-based diagnostics solidify its foundational role in CRISPR-driven molecular sensing platforms. Altogether, these advances position Cas9 as both a pioneering genome editor and a versatile molecular sensor at the forefront of CRISPR-Dx.

4.2. Cas12

The CRISPR-Cas12 system has emerged as a pivotal tool for nucleic acid diagnostics due to its unique dual-mode

NUC activity. Upon REC of a target DNA sequence flanked by a 5'-TTTV-3' PAM, Cas12a undergoes conformational activation and initiates DSBs via its RuvC domain.¹⁷⁶ Notably, this activation also triggers a robust trans-cleavage mechanism, whereby Cas12a indiscriminately cleaves nearby ssDNA. This property enables signal amplification in diagnostic platforms through cleavage of labeled reporter molecules, a feature not present in Cas9, and is highly advantageous for sensitive and rapid detection.^{177,178}

Furthermore, Cas12a's molecular versatility has been harnessed in a range of detection formats. The DETECTR assay, developed during the COVID-19 pandemic, combined reverse transcription loop-mediated isothermal amplification (LAMP) with Cas12a-mediated detection of SARS-CoV-2 in clinical nasopharyngeal samples, producing results in under 30–45 min, with 95% positive predictive agreement and 100% negative predictive agreement, directly visualized through lateral flow readouts.¹⁷⁹ The schematic in **Figure 4** illustrates a CRISPR-Cas12a-based diagnostic approach that integrates nucleic acid detection with a lateral flow assay for rapid and sensitive diagnostics. In oncology, Yu *et al.*¹⁸⁰ engineered an amplification-free Cas12a-based electrochemiluminescent biosensor incorporating DNA tetrahedron nanostructures

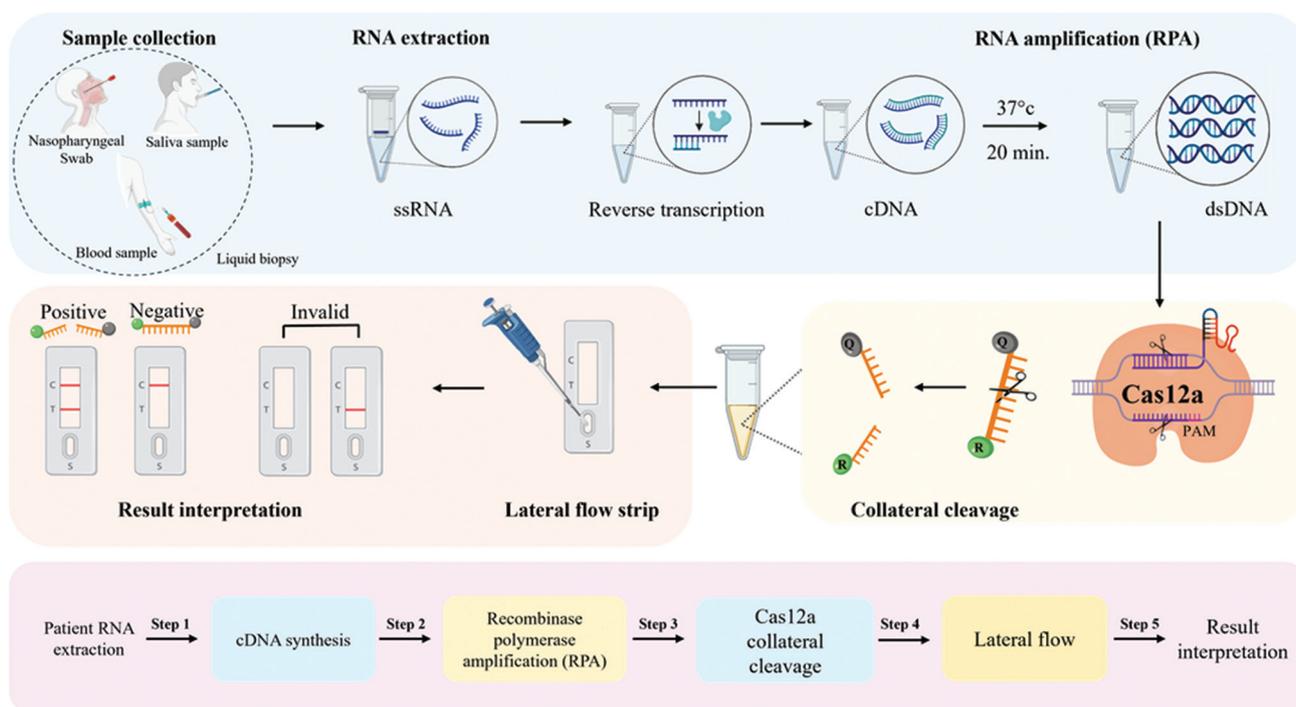


Figure 4. Schematic representation of a CRISPR–Cas12a-based diagnostic approach that integrates nucleic acid detection with a lateral flow assay for rapid and sensitive diagnostics. The process begins with sample collection, where nasopharyngeal swabs, saliva, or blood—part of a liquid biopsy—are obtained from patients. Step 1 involves RNA extraction to isolate ssRNA, which is then reverse transcribed into cDNA. In Step 2, the cDNA undergoes RPA at 37°C for 20 minutes, generating dsDNA to enrich the target sequence. Step 3 introduces the amplified DNA to Cas12a, which, upon recognizing the specific target sequence, activates its collateral cleavage activity, indiscriminately cutting nearby single-stranded reporter probes labeled with a fluorophore and quencher. In Step 4, the cleaved reporter probes are applied to a lateral flow strip, initiating visual detection. Finally, Step 5 involves result interpretation, where the test strip is analyzed based on the appearance of test and control lines, to determine whether the outcome is positive, negative, or invalid. This approach provides an efficient and accurate nucleic acid detection platform, making it ideal for point-of-care diagnostics. Figure created by the authors.

Abbreviations: Cas: CRISPR-associated protein; cDNA: Complementary DNA; CRISPR: Clustered regularly interspaced short palindromic repeats; dsDNA: Double-stranded DNA; PAM: Protospacer adjacent motif; ssRNA: Single-stranded RNA.

for the amplification-free detection of human papillomavirus (HPV)-16, achieving a detection limit of 8.86 fM within a 100-min workflow. Similarly, Luo *et al.*¹⁸¹ reported a nanobeacon-driven Cas12a sensor for direct microRNA (miRNA)-21 detection within five minutes, bypassing the need for reverse transcription and illustrating Cas12a's ability to detect non-coding RNAs in complex samples.

Beyond these applications, Cas12a has been used to detect bacterial and environmental pathogens. A dual-mode biosensor integrating fluorescence and electrochemical readouts successfully identified *Staphylococcus aureus* using a Cas12a-triggered hybridization chain reaction, with a detection limit of 5.7 CFU/mL.¹⁸² Similarly, for tuberculosis diagnostics, an electrochemical Cas12a sensor targeting the *IS6110* gene of *Mycobacterium tuberculosis* achieved a detection limit of 14.5 nM through voltammetry within 60 min.¹⁸³ In addition, Cas12a-based biosensors have been adapted to detect resistance-associated mutations in *M. tuberculosis*, enabling genotypic identification of drug-resistant strains such as multidrug-resistant tuberculosis.¹⁸⁴ Companies like Mammoth Biosciences have integrated Cas12-based DETECTR platforms into pathogen-specific diagnostics, enabling rapid, point-of-care detection of infectious agents, including tuberculosis (Table 6). These biosensors facilitate

rapid treatment stratification in clinical settings and address critical gaps left by slow, culture-based drug susceptibility tests. Moreover, Cas12a-based biosensing has also been applied to antibiotic monitoring; a fluorescence aptasensor for ampicillin, using Cas12a-cleavable ssDNA reporters, reached a detection threshold of 0.01 nM within 30 min, even in spiked food samples.¹⁸⁵ In several contexts, Cas12a has been coupled with recombinase polymerase amplification (RPA) and rolling circle amplification (RCA) for the sensitive detection of *Escherichia coli* in water and food samples. For instance, a dual fluorescence/lateral flow RPA-Cas12a assay detected *E. coli* O157:H7 down to 1.8 fg/μL (\approx 2.4 CFU/mL) within 40 min, while an RCA-Cas12a electrochemical biosensor achieved attomolar-level predictive sensitivity.¹⁸⁶

Mechanistically, Cas12a's trans-cleavage activity allows for single-molecule detection, high turnover rates, and flexibility in signal design. Its compatibility with isothermal amplification (RPA, LAMP) and tolerance to variable reaction conditions make it highly suited for point-of-care and field-deployable diagnostic systems.²⁰⁷ Importantly, the programmability of its gRNAs and its broad modality compatibility—fluorescent, electrochemical, and lateral flow—position Cas12a as a diagnostic effector of exceptional breadth, enabling the detection of viral RNA, tumor DNA, bacterial

Table 6. Leading CRISPR-Cas companies: Focus areas in diagnostics, prognostics, and biosensing

Company name	CRISPR variant (s)	Primary diagnostic focus/platforms	Detection method	Key features/notes	References
Diagnosis					
SHERLOCK Biosciences	Cas13a, Cas12a	Infectious diseases (e.g., SARS-CoV-2, tuberculosis, malaria), genetic mutations	Fluorescence, lateral flow	Pioneers of the SHERLOCK platform; high sensitivity; POC ready	<a href="https://sherlock.bio<sup>187</sup>">https://sherlock.bio¹⁸⁷
Mammoth Biosciences	Cas12a, Cas14, CasΦ	Infectious diseases (e.g., SARS-CoV-2), genetic conditions	Lateral flow, fluorescence	Co-founded by Nobel laureate Jennifer Doudna; develops the DETECTR platform; supports multiplexing and portable diagnostics	<a href="https://mammoth.bio<sup>188</sup>">https://mammoth.bio¹⁸⁸
CrisprBits	Cas12a, Cas13a	Infectious diseases (e.g., SARS-CoV-2 Omicron variant, other GI tract infections), antimicrobial resistance genes	Lateral flow, electrochemical	Indian company developing affordable and accessible CRISPR-based diagnostics; low-cost; community surveillance and environmental testing	<a href="https://crisprbits.com<sup>189</sup>">https://crisprbits.com¹⁸⁹
Caspr Biotech	Cas12a, Cas13a	Molecular diagnostics (various applications), COVID-19	Paper-based strip, RT-RPA	Portable and accurate CRISPR-based diagnostics; diverse applications	<a href="https://sosv.com/company/caspr-biotech/<sup>190</sup>">https://sosv.com/company/caspr-biotech/¹⁹⁰
Scope Biosciences	Cas12a	Molecular diagnostics	Fluorescence, LAMP	Dutch biotech firm; high specificity; pathogen and mutation detection	<a href="https://scopebio.com<sup>191</sup>">https://scopebio.com¹⁹¹
Locus Biosciences	Cas3	Precision antibacterial (bacterial infections)	Bacteriophage-mediated	Uses CRISPR-Cas3 bacteriophage (crPhage) technology to degrade bacterial DNA	<a href="https://www.locus-bio.com<sup>192</sup>">https://www.locus-bio.com¹⁹²
Medic Life Sciences	Cas9, Cas12a	Cancer biomarkers, drug discovery	Fluorescent, CRISPR screens	Functional genomics to identify and validate cancer targets	<a href="https://www.medic-life-sciences.com<sup>193</sup>">https://www.medic-life-sciences.com¹⁹³
Integrated DNA Technologies (IDT)	Cas9, Cas12a, Cas13a	Reagents and tools for CRISPR diagnostics	Enabling reagents	Supports R&D; major reagent supplier for diagnostic developers	<a href="https://sg.idtdna.com/page/products/crispr-genome-editing<sup>194</sup>">https://sg.idtdna.com/page/products/crispr-genome-editing¹⁹⁴
Thermo Fisher Scientific	Cas9, Cas12a	Reagents, kits, and platforms for CRISPR research and diagnostics	Multiplex PCR, qPCR, LAMP	Supplies instruments and kits for CRISPR R&D workflows	<a href="https://www.thermofisher.com/in/en/home/life-science/genome-editing/crispr-nuclease-vector.html<sup>195</sup>">https://www.thermofisher.com/in/en/home/life-science/genome-editing/crispr-nuclease-vector.html¹⁹⁵
Takara Bio Inc.	Cas9, Cas12a	Molecular diagnostics, gene therapy	LAMP, RT-qPCR	Japanese biotechnology company specializing in genome editing, gene therapy, and diagnostics; Asia-Pacific leader	<a href="https://www.takarabio.com/?srsltid=AfmBOooCQFJ7Nuv1BZef22CUGhEXW_jNCJnuSuoi36BrSTTcaw1aDne0<sup>196</sup>">https://www.takarabio.com/?srsltid=AfmBOooCQFJ7Nuv1BZef22CUGhEXW_jNCJnuSuoi36BrSTTcaw1aDne0¹⁹⁶
Prognosis					
Academic/research institutions (e.g., Broad Institute, UC Berkeley)	Cas9, Cas12a	Discovery of prognostic gene signatures, drug resistance biomarkers	Genome-wide knockout/activation screens	Pioneers in CRISPR-based prognostic screening	<a href="https://www.broadinstitute.org/crispr/information-about-crispr-cpf1-cas12a-systems<sup>197</sup>">https://www.broadinstitute.org/crispr/information-about-crispr-cpf1-cas12a-systems¹⁹⁷
Companies with strong diagnostic platforms (e.g., SHERLOCK Biosciences, Mammoth Biosciences)	Cas13a, Cas12a	Prognostic biomarker detection, monitoring disease progression	SHERLOCK assay, isothermal amplification	Enables detection of relapse and recurrence; focuses on real-time, low-abundance biomarker detection	https://sherlock.bio <a href="https://mammoth.bio<sup>187,188</sup>">https://mammoth.bio^{187,188}

(Cont'd...)

Table 6. (Continued)

Company name	CRISPR variant (s)	Primary diagnostic focus/ platforms	Detection method	Key features/notes	References
Companies focused on precision oncology/ drug discovery (e.g., Repare Therapeutics, KSQ Therapeutics)	Cas9	Identification of drug response biomarkers, overcoming drug resistance	Functional CRISPR screens	Precision oncology targeting vulnerabilities	https://www.reparerx.com https://ksqtx.com ^{198,199}
Crown Bioscience	Cas9	Predictive biomarker identification for drug discovery	CRISPR-edited tumor models	Identifies treatment response profiles in oncology	https://www.crownbio.com ²⁰⁰
Takara Bio Inc.	Cas9, dCas9	Tools and services for biomarker discovery	Custom screen libraries	Supports multiplexed CRISPR-based diagnostics	https://www.takarabio.com/?srsltid=AfmBOooCQFJ7Nuv1BZef22CUGhEXW_jNCJnuSuoi36BrSTTcaw1aDne0 ¹⁹⁶
Companies Developing Liquid Biopsy Solutions (CRISPR-enhanced)	Cas12a, Cas13a	Detection of circulating prognostic biomarkers	Microfluidics-integrated CRISPR detection	Focused on non-invasive prognosis solutions	https://www.freenome.com https://guardanthealth.com https://www.natera.com ²⁰¹⁻²⁰³
Biosensing					
Mammoth Biosciences	Cas12a, Cas14, CasΦ	Broad molecular diagnostics (healthcare, environmental)	DETECTR, isothermal amplification	Leading player in CRISPR diagnostics; aims to create a “programmable diagnostic platform” for any biomarker	https://mammoth.bio ¹⁸⁸
SHERLOCK Biosciences	Cas13a, Cas12a	Infectious disease diagnostics (POC)	SHERLOCK, LFA, RPA	Rapid and affordable POC diagnostics using RNA/DNA sensing; strong COVID-19 and STI testing portfolio; acquired by OraSure Technologies (2024)	https://sherlock.bio ¹⁸⁷
Cardea Bio	Cas9, dCas9	Integrated biosensors (CRISPR-Chip)	CRISPR-Chip (electronic detection)	Label-free, real-time sensing of nucleic acids; integrates CRISPR with electronics; useful in continuous monitoring and environmental biosensing	https://www.serraventures.com/cardea-bio-1 ²⁰⁴
CrisprBits	Cas12a	Affordable diagnostics (developing nations focus)	OmiCrisp (paper-based), fluorescence	Focused on SARS-CoV-2 variants and AMR detection; cost-effective platform for India; exploring food/agriculture applications	https://crisprbits.com ¹⁸⁹
Proof Diagnostics	Cas12a	Rapid COVID-19 diagnostics	Fluorescent LFA	Developed during the pandemic for at-home testing; demonstrates CRISPR's agility in emergency diagnostic development	https://www.ginkgo.bio ²⁰⁵
Caribou Biosciences	Cas9, chRDNA	Broader genomics and potential diagnostics	CRISPR-Cas screens	Primarily therapeutics-focused; exploring diagnostics using engineered Cas proteins for broad detection and high-throughput applications	https://www.cariboubio.com ²⁰⁶

(Cont'd...)

Table 6. (Continued)

Company name	CRISPR variant(s)	Primary diagnostic focus/platforms	Detection method	Key features/notes	References
Thermo Fisher Scientific	Cas9, Cas12a	CRISPR reagents and platforms (enabler)	qPCR-compatible, isothermal platforms	Supplies critical reagents and kits; not a biosensor firm per se, but supports CRISPR-based detection R&D globally	https://www.thermofisher.com/in/en/home/life-science/genome-editing/crispr-nuclease-vector.html ¹⁹⁵

Abbreviations: AMR: Antimicrobial resistance; CRISPR-Cas: Clustered regularly interspaced short palindromic repeats and CRISPR-associated protein; dCas9: Catalytically inactivated Cas9; DETECTR: DNA endonuclease-targeted CRISPR trans reporter; GI: Gastrointestinal; LAMP: Loop-mediated isothermal amplification; LFA: Lateral flow assay; POC: Point-of-care; qPCR: Quantitative polymerase chain reaction; RPA: Recombinase polymerase amplification; RT: Real-time; R&D: Research and development; SHERLOCK: Specific High-sensitivity Enzymatic Reporter unLOCKing; STI: Sexually transmitted infection.

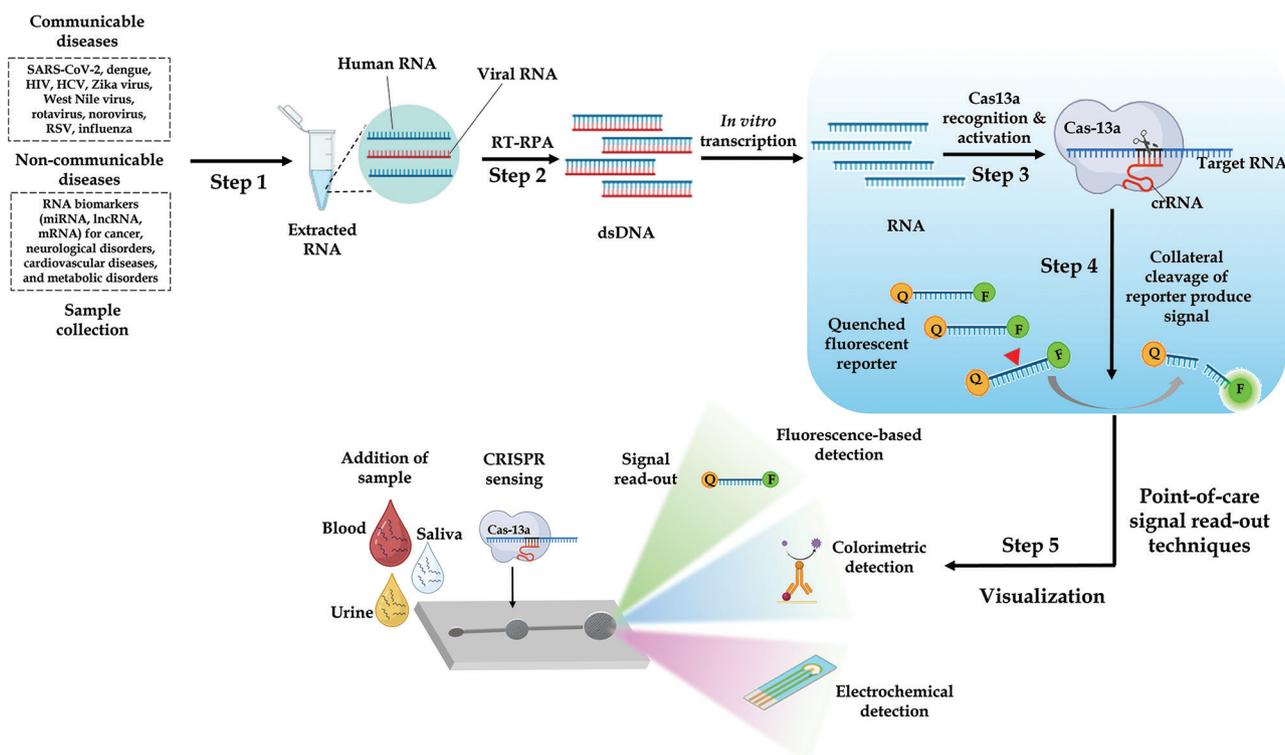


Figure 5. CRISPR–Cas13a-based nucleic acid detection workflow. Step 1 involves nucleic acid extraction from the sample. In Step 2, isothermal amplification methods, such as RPA, enhance detection sensitivity by increasing the target RNA concentration. Step 3 illustrates the Cas13a–crRNA complex binding to the target RNA, resulting in its activation. In Step 4, the activated Cas13a enzyme exhibits collateral cleavage activity, cutting not only the target RNA but also surrounding RNA, including a quenched fluorescent reporter. Step 5 highlights the detection phase, where the cleavage of the reporter RNA generates a detectable signal. This signal can be visualized using various modalities, including fluorescence-based detection, colorimetric assays, and electrochemical sensors—offering versatile, sensitive, and specific diagnostic capabilities. Figure created by the authors.

Abbreviations: Cas: CRISPR-associated protein; CRISPR: Clustered regularly interspaced short palindromic repeats; crRNA: CRISPR RNA; dsDNA: Double-stranded DNA; HCV: Hepatitis C virus; lncRNA: Long non-coding RNA; mRNA: Messenger RNA; miRNA: MicroRNA; RPA: Recombinase polymerase amplification; RSV: Respiratory syncytial virus.

genomes, miRNAs, and chemical contaminants across clinical, environmental, and industrial domains.

4.3 Cas13

The CRISPR-Cas 13 system is unique in targeting RNA rather than DNA, using crRNA-guided REC to activate its dual higher eukaryotes and prokaryotes nucleotide-binding NUC domains for both specific target cleavage and non-specific trans-cleavage of surrounding ssRNA.²⁰⁸ This collateral cleavage activity accounts for its remarkable diagnostic

sensitivity, often reaching attomolar limits, making Cas13 a powerful tool for RNA pathogen detection, miRNA profiling, and transcriptomic diagnostics.²⁰⁹ Cas13-centered diagnostics are exemplified by the SHERLOCK platform, which integrates real-time RPA amplification and Cas13a-mediated reporter cleavage.²¹⁰ **Figure 5** illustrates the workflow of nucleic acid detection based on CRISPR-Cas13a, emphasizing its versatility and specificity. It was quickly adapted for SARS-CoV-2 detection and later extended to other pathogens. Notably, SHERLOCK has been refined to detect infectious bursal disease

virus with a 5 aM limit, delivering superior sensitivity to real-time PCR across 70 field samples.²¹¹ Sherlock Biosciences, which pioneered the SHERLOCK system, continues to expand CRISPR-Cas13 applications to cover a broad spectrum of infectious and antimicrobial resistance diagnostics (Table 6). For mosquito-borne illnesses, a malaria-specific SHERLOCK assay using LwCas13a enables simultaneous *Plasmodium* species identification and drug-resistance single-nucleotide variant (SNV) genotyping in a multiplexed reaction, demonstrating field-compatible precision.²¹² Similarly, Cas13-based diagnostics have been employed to detect resistance-associated mutations in HIV, offering rapid genotypic insights for guiding antiretroviral therapy.²¹³ By targeting specific RNA regions linked to drug resistance, these assays outperform conventional PCR in detecting low-abundance variants, making them valuable for real-time treatment decisions in clinical and low-resource settings. Notably, a rapid isothermal Cas13a-based kit for genital herpes simplex virus achieved near-perfect sensitivity and specificity (96.2% and 100%, respectively), with a 1 copy/ μ L detection threshold in a 194-sample clinical cohort.²¹⁴

In oncology, the Cas-catalyzed hairpin DNA circuit electrochemical biosensor (COMET) utilizes Cas13a collateral cleavage followed by a catalytic hairpin DNA circuit to reliably quantify multiple non-small cell lung carcinoma-associated RNAs, including miR-17, miR-155, miR-19b, and miR-210, with a dynamic range from 50 aM to 5 nM.²¹⁵ It differentiated early-stage cancer patients from controls within 36 min using only 10 μ L of serum. Furthermore, for direct, amplification-free miRNA profiling, photoelectrochemical and microfluidics-enabled electrochemical sensors incorporated Cas13a to detect miRNA-21 and other non-coding RNAs in <10 min with picomolar sensitivity.²¹⁶ Such modalities highlight Cas13's adaptability to highly sensitive RNA-targeted detection. Mechanistically, Cas13-based diagnostics thrive due to collateral cleaving of ssRNA reporters, precise single-base mismatch discrimination (especially for SNV detection), PAM-independent targeting flexibility, and multiplexing options through orthogonal reporter designs.²¹⁷ Combined with isothermal amplification techniques like real-time RPA/LAMP or even in amplification-free formats, Cas13 assays combine high specificity, rapid performance, and simple hardware compatibility, making them prime candidates for both field-based infectious disease surveillance and precision diagnostics in oncology and genetic research.²¹⁸

4.4. Cas14

Cas14, also referred to as Cas12f, represents one of the most compact CRISPR-associated NUCs, measuring only ~400–700 amino acids.¹⁰⁰ First discovered by Jennifer Doudna's group in 2018, Cas14 exhibits a unique combination of features that distinguish it from Cas9, Cas12, and Cas13 effectors. It targets ssDNA with high specificity and performs both cis- and trans-cleavage without requiring a PAM, offering exceptional flexibility in sequence REC.¹⁵² These attributes make it an attractive candidate for diagnostic and genome engineering applications, particularly where space-constrained delivery systems or highly sensitive detection are required.²¹⁹

Figure 6 illustrates Cas14a-mediated DNA cleavage mechanisms, showing its cis- and trans-cleavage activities for enhanced genome-editing precision.

Mechanistically, Cas 14 is guided by a crRNA to recognize ssDNA targets, on which it activates trans-cleavage of surrounding non-target ssDNA molecules, a property similar to Cas12a and Cas13 but executed with higher substrate selectivity and in a PAM-independent manner. This molecular precision and low background activity make Cas14 highly suitable for integration into biosensors that depend on signal amplification through reporter cleavage. Its minimal size further facilitates incorporation into point-of-care and microfluidic diagnostic devices, where compact delivery is essential.^{220,221} Several biosensing strategies have successfully employed Cas14a for nucleic acid and small molecule detection. For example, Wang *et al.*²²² developed a photoelectrochemical biosensor combining Cas14a with upconversion nanoparticles and SDA to detect T-2 toxin in oats and protein kinase PTK7 in human serum. This sensor achieved femtogram-level sensitivity and demonstrated high specificity in complex biological matrices. Similarly, a primer exchange reaction (PER)-Cas14a electrochemical biosensor has been engineered for circulating tumor DNA detection, including epidermal growth factor receptor (EGFR) *L858R* mutations associated with non-small cell lung cancer.²²³ This platform achieved a detection limit of 0.34 fM and a broad dynamic range, showing strong potential for liquid biopsy applications. Cas14a has also been applied in pathogen diagnostics. In one study, an electrochemical sensor integrating Cas14a with PtPd@PCN-224 nanoenzymes enabled ultra-sensitive detection of *Burkholderia pseudomallei*, with a detection limit of just 12.8 aM.²²⁴

In a different context, the highly sensitive Aptamer-Regulated R-loop for bioanalysis system utilized Cas14a's collateral activity for aptamer-guided detection of various small molecules, including adenosine triphosphate (ATP), histamine, cadmium, and thrombin. This system provided nanomolar sensitivity in a label-free format and demonstrated broader versatility than comparable Cas12a-based approaches.^{225,226} Importantly, Cas14a's diagnostic potential has attracted the attention of industry, with Mammoth Biosciences actively engineering Cas14 variants for portable, rapid, and equipment-free diagnostic platforms.²²⁷ Their development focus includes lateral flow systems and CRISPR-integrated paper devices that can operate in decentralized, low-resource settings—features crucial for global infectious disease surveillance and mobile diagnostics. Despite its advantages, Cas14 still faces several translational challenges. Its activity can be sensitive to temperature fluctuations, and its ssDNA-targeting nature limits broader genomic applications unless modified or paired with upstream amplification strategies.²²⁸ In addition, further studies are needed to evaluate off-target effects, enzyme kinetics, and real-world performance in clinical samples. Nonetheless, Cas14a's compact size, PAM independence, and collateral cleavage capability position it as a powerful next-generation CRISPR effector for precision diagnostics and synthetic biosensor systems.

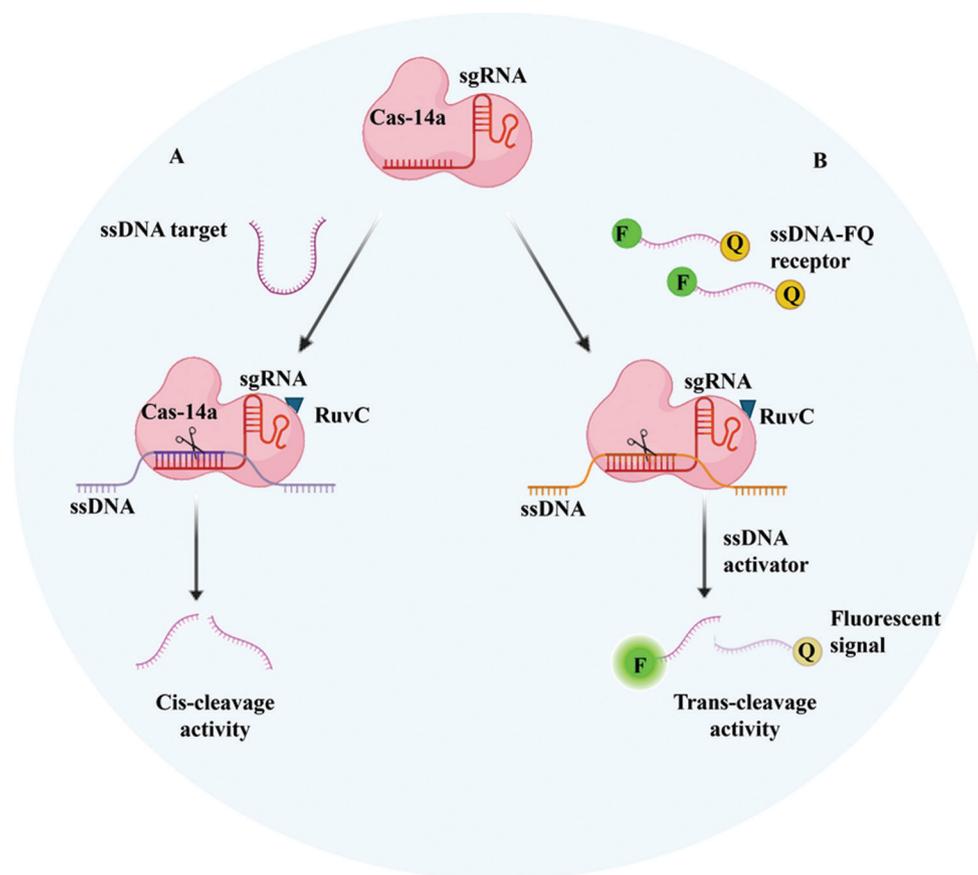


Figure 6. Cas14a-mediated DNA cleavage mechanisms. The Cas14a protein binds to an sgRNA and recognizes an ssDNA target. Upon binding, Cas14a exhibits two types of cleavage activities: (A) Cis-cleavage activity, where the target ssDNA is directly cleaved at the binding site by the RuvC domain; and (B) Trans-cleavage activity, which is triggered upon recognition of an ssDNA activator. This results in the cleavage of surrounding ssDNA substrates, including an FQ-labeled ssDNA reporter, leading to the release of a fluorescent signal. This signal serves as an indicator of Cas14a activation and target DNA recognition. Figure created by the authors.

Abbreviations: Cas: CRISPR-associated protein; FQ: Fluorescence-quencher; RuvC: RecU-like resolvase; sgRNA: Single guide RNA; ssDNA: Single-stranded DNA.

5. Programmable CRISPR-based biosensors

Biosensing is a multidisciplinary approach that detects biological molecules by combining a biorecognition element, such as enzymes or nucleic acids, with a signal transducer that converts biological interactions into measurable signals.²²⁹ Among emerging technologies, CRISPR-Cas systems have rapidly gained prominence as programmable biosensing platforms, offering precise, portable, and adaptable solutions for molecular diagnostics.¹⁰¹ In these biosensors, Cas effectors are directed by synthetic gRNAs to identify specific nucleic acid targets, whereupon signal generation occurs through mechanisms such as collateral cleavage, binding-induced changes, or enzymatic activation.¹⁷⁸ CRISPR-based biosensors differ fundamentally from conventional techniques such as PCR, ELISA, or NGS by providing amplification-free, isothermal, and real-time detection capabilities, often used at the point-of-care.²³⁰ Platforms such as CRISPR-Chip, which integrates dCas9 with a graphene field-effect transistor, enable label-free and portable detection of DNA mutations, offering clinical applications in cancer and genetic disorders.²³¹ Cas effectors, including Cas9, Cas12, Cas13, and Cas14, have been tailored into biosensor designs, each contributing distinct molecular properties.⁹⁸ For example, Cas13-based SHERLOCK

and Cas12-based DETECTR systems exploit collateral cleavage for sensitive, programmable nucleic acid detection.²³²

Figure 7 compares DETECTR and SHERLOCK technologies, showcasing their distinct enzymatic activities and diagnostic applications. Beyond nucleic acids, CRISPR biosensors are being adapted to detect proteins and small molecules through aptamer fusion and hybrid REC elements.²³³ Miniaturization strategies such as microfluidic integration, paper-based assays, and smartphone-compatible readouts are driving the development of field-deployable CRISPR diagnostics.²³⁴ These biosensors are being engineered to detect pathogens such as SARS-CoV-2 and Zika virus, cancer-associated mutations such as *EGFR* and *KRAS*, and metabolic biomarkers for diseases including diabetes and cardiovascular disorders.^{235,236} Despite their promise, CRISPR biosensors face limitations, including off-target effects, scalability constraints, and the need for regulatory validation.²³⁷ Continued advancements in enzyme engineering, gRNA optimization, and multiplex signal design are enhancing the specificity, sensitivity, and clinical robustness of these platforms.²³⁸ Notably, integrating CRISPR with aptamer REC, nanostructures, electrochemical sensors, and fluorescent or bioluminescent reporters has led to a new generation of multiplexed, low-cost biosensing solutions.²³⁹

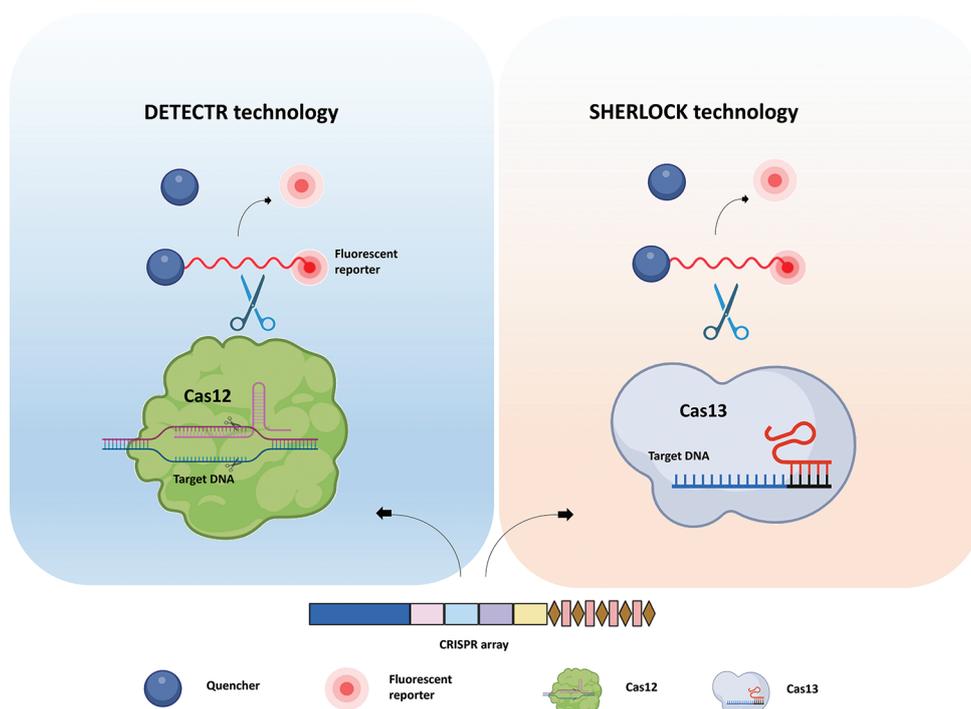


Figure 7. Comparison between DETECTR and SHERLOCK technologies. The left panel illustrates DETECTR, which utilizes the Cas12 enzyme guided by a crRNA to bind to a specific target DNA sequence. Upon successful target recognition, Cas12 exhibits collateral cleavage activity on single-stranded DNA, leading to the degradation of a fluorescent reporter molecule and generation of a detectable signal. In contrast, the right panel depicts SHERLOCK, which is based on the Cas13 enzyme. Cas13 is similarly guided by crRNA to recognize a target RNA sequence. Upon binding, Cas13 activates its collateral RNA cleavage activity, resulting in the breakdown of a fluorescently labeled RNA reporter and the production of a detectable signal. Both technologies leverage the collateral cleavage activity of Cas enzymes to enable precise and sensitive nucleic acid detection. The bottom legend identifies key molecular components involved in both methods, including fluorescent reporters, target DNA, Cas enzymes (Cas12 for DETECTR and Cas13 for SHERLOCK), and guide RNA sequences. These CRISPR-based platforms have revolutionized molecular diagnostics by enabling rapid, precise, and portable detection of pathogens and genetic variations. Figure created by the authors.

Abbreviations: Cas: CRISPR-associated protein; CRISPR: Clustered regularly interspaced short palindromic repeats; crRNA: CRISPR RNA; DETECTR: DNA endonuclease targeted CRISPR trans reporter; SHERLOCK: Specific High-sensitivity Enzymatic Reporter unLOCKing.

This section provides a comprehensive overview of diverse CRISPR biosensor architectures, beginning with CRISPR-Cas12a (cpf1)-based electrochemical biosensors (E-CRISPR) and expanding through colorimetric, fluorescence-based, bioluminescent, aptamer-assisted, and nanotechnology-enabled platforms. These modular diagnostic systems exemplify how CRISPR effectors are redefining biosensing at the molecular level and enabling precision diagnostics in both laboratory and field settings. Several companies are actively developing these platforms. For example, Sherlock Biosciences has pioneered the SHERLOCK platform for rapid detection of infectious agents using Cas13 enzymes, while Mammoth Biosciences has developed the DETECTR system, leveraging Cas12 and Cas14 enzymes for portable, highly sensitive diagnostics. Companies such as CrisprBits, Caspr Biotech, and Scope Biosciences are also contributing to global CRISPR biosensing innovation, targeting both healthcare and environmental applications (Table 6).

5.1. E-CRISPR

E-CRISPR is an innovative biosensing platform that integrates the sensitivity and miniaturization potential of electrochemical transduction with the nucleic acid REC and

cleavage capabilities of CRISPR to identify specific DNA or RNA sequences.²⁴⁰ Unlike fluorescence- or colorimetric-based assays, which rely on optical signals, E-CRISPR detects biomolecular interactions by quantifying electrical changes—such as current, potential, or impedance—induced by CRISPR-mediated cleavage or binding events.²⁴¹ This strategy enables portable, low-cost, and label-free detection, making it particularly well-suited for point-of-care diagnostics in both clinical and field settings.²⁴² Mechanistically, an E-CRISPR platform typically incorporates a gold- or carbon-based working electrode modified with capture probes specific to the target nucleic acid.²⁴³ Upon introduction of the CRISPR complex, most often Cas12a or Cas13a paired with a predesigned gRNA, the system recognizes the target sequence.²⁴⁴ Furthermore, the binding induces activation of the NUC, triggering collateral or target-specific cleavage of nearby ssDNA reporter strands attached to the electrode surface.²⁴⁵ This cleavage disrupts the electrochemical interface, leading to quantifiable signal shifts measured by differential pulse voltammetry, square wave voltammetry, or electrochemical impedance spectroscopy.^{246,247} In one notable application, a Cas12a-based E-CRISPR biosensor was developed for the rapid detection of HPV-16, a high-risk oncogenic strain of HPV.²⁴⁸ The sensor

achieved picomolar-level sensitivity in blood and cervical swab samples and delivered results within an hour, underscoring its potential for real-time, resource-limited diagnostics.²⁴⁹ In another design, researchers engineered an amplification-free E-CRISPR system integrating DNA tetrahedron nanostructures and aptamer-conjugated electrodes, enabling signal amplification without enzymatic pre-processing.²⁵⁰ The versatility of E-CRISPR has also been extended to detect small molecules and proteins by combining CRISPR REC with aptamer-based molecular switches.²⁵¹ These hybrid designs further expand the utility of electrochemical biosensors beyond nucleic acids, accommodating a broader range of diagnostic biomarkers. Importantly, electrochemical sensors can be miniaturized for integration into wearable or handheld devices, enhancing accessibility in remote or under-resourced regions. Despite their advantages, these platforms face challenges, including standardization of surface functionalization, potential nonspecific adsorption, and regulatory oversight regarding CRISPR usage.²⁵² However, ongoing innovations in nanostructured electrodes, microfluidic interfacing, and CRISPR enzyme engineering continue to improve signal fidelity and clinical translatability. As such, electrochemical CRISPR biosensors are emerging as powerful tools for rapid, accurate, and decentralized molecular diagnostics.

5.2. Colorimetry-CRISPR biosensors

Colorimetry-CRISPR biosensors are a class of diagnostic platforms that translate CRISPR-mediated nucleic acid REC into visible color changes, allowing rapid, equipment-free detection of specific genetic targets.²⁵³ These systems leverage the cleavage activity of Cas12 or Cas13 effectors on ssDNA or RNA reporters labeled with chromogenic substrates, producing a colorimetric signal that can be seen with the naked eye.²⁵⁴ This simplicity makes colorimetric CRISPR diagnostics especially well-suited for low-resource, point-of-care settings, where access to advanced fluorescence or electrochemical instrumentation is limited.²⁵⁵ Mechanistically, colorimetric detection relies on collateral cleavage: when Cas12 or Cas13 is activated by binding to a target sequence, it nonspecifically cleaves nearby reporter molecules.²⁵⁶ These reporters are often linked to gold nanoparticles (AuNPs), horseradish peroxidase, or G-quadruplex/hemin complexes, which generate a visible signal shift upon structural disruption.²⁵⁷ For instance, in AuNP-based systems, cleaved DNA linkers result in nanoparticle dispersion or aggregation, causing a distinct color change from red to purple, or vice versa, depending on the assay design.²⁵⁸ A well-established application of this technology is the detection of SARS-CoV-2 using Cas12a, where viral RNA is reverse transcribed and amplified using isothermal methods such as RPA.²⁵⁹ The amplified product then activates Cas12a, which cleaves ssDNA-labeled reporters, producing a color change that correlates with viral presence.²⁶⁰ Such assays have demonstrated comparable sensitivity to real-time PCR in field validation studies, with results visible within 30–60 min.²⁶¹ Beyond infectious diseases, colorimetric CRISPR platforms are also being explored for early cancer diagnostics.²⁶² For example, CRISPR-Cas13a-based colorimetric assays have been developed for miRNA

detection in plasma samples, allowing identification of key biomarkers such as miR-21, often overexpressed in non-small cell lung carcinoma.²⁰⁹ These platforms use catalytic hairpin assembly and G-quadruplex-based color generation, offering high sensitivity without the need for fluorescent probes.²⁶³ The portability, low cost, and ease of interpretation offered by colorimetric CRISPR biosensors make them especially attractive for decentralized diagnostics, including community health programs, rural clinics, and emergency outbreak response.^{264,265} However, challenges remain in terms of signal quantification, multiplexing capability, and the shelf-stability of reagents under varied environmental conditions.²⁵² As research progresses, improvements in nanozyme integration, stabilized chromogenic substrates, and multiplex color-code readouts are expected to broaden the clinical applicability of colorimetry-CRISPR biosensors. These developments position them as promising diagnostic tools in efforts to achieve universal, rapid, and affordable disease detection globally.

5.3. Fluorescence and bioluminescence-based biosensors

Fluorescence and bioluminescence-based CRISPR biosensors provide highly sensitive, real-time platforms for nucleic acid detection and molecular imaging.²⁶⁶ These systems translate CRISPR-mediated target REC into light-based signals, using either externally excited fluorophores or internally generated bioluminescent reporters.²⁶⁷ This capability allows researchers and clinicians to monitor dynamic biological events *in vitro* and *in vivo* with high precision, making these platforms valuable not only for molecular diagnostics but also for live-cell imaging and personalized therapy monitoring. Fluorescent CRISPR biosensors typically use Cas12 or Cas13 proteins coupled with reporter probes labeled with a fluorophore and quencher.²⁶⁸ Upon activation by a target sequence, the Cas effector cleaves the reporter, separating the fluorophore from the quencher and producing a measurable fluorescent signal.²⁶⁹ Furthermore, fluorogenic probes such as quantum dots, carbon dots, and fluorescence resonance energy transfer (FRET) pairs enable multiplexed detection and high signal-to-noise ratios.²⁷⁰⁻²⁷² Luminescence resonance energy transfer, an advanced variant of FRET, utilizes lanthanide donors for distance-based molecular measurements, offering improved photostability and reduced background interference, ideal for intracellular sensing applications.²⁷³ To enhance sensitivity, these biosensors are often combined with isothermal amplification techniques, which enable nucleic acid amplification at a constant temperature without the need for thermal cycling.²⁷⁴ Techniques such as RPA, LAMP, SDA, and NASBA are frequently integrated into CRISPR fluorescence workflows.²⁷⁵⁻²⁷⁸ These combinations enable ultra-sensitive detection of genetic material even at attomolar levels. In addition, the SHERLOCK and DETECTR platforms are landmark examples of fluorescence-based CRISPR diagnostics.^{279,280} SHERLOCK uses Cas13a with fluorescent RNA reporters to detect RNA viruses such as Zika and SARS-CoV-2, while DETECTR uses Cas12a with ssDNA-fluorescence-quencher probes for DNA-based pathogens and mutations, including HPV.^{281,282} Notably, bioluminescence-based CRISPR biosensors differ from fluorescence-based systems in that they

do not require external excitation.²⁸³ Instead, they employ luciferase-based systems that emit light through enzymatic oxidation reactions.²⁸⁴ These platforms are gaining traction for *in vivo* imaging and cancer diagnostics, where real-time, non-invasive monitoring of tumor progression is essential. For instance, bioluminescent CRISPR reporters have been used to monitor tumor metastasis, immune cell infiltration, and therapeutic response in mouse models, providing dynamic insights into disease biology.²⁸⁵ Furthermore, researchers have developed hybrid systems combining CRISPR-Cas9 with split luciferase complementation assays, enabling the detection of target sequences through reconstituted light emission.²⁸⁶ These approaches have been applied in tracking gene-editing outcomes, validating gRNA activity, and imaging CRISPR dynamics within living tissues. Despite their advantages, fluorescence- and bioluminescence-based CRISPR biosensors face challenges in instrumentation requirements, signal stability, and background interference, particularly in complex biological matrices.²²⁵ Nevertheless, continuous improvements in reporter chemistry, enzyme engineering, and signal amplification are addressing these limitations and paving the way for real-time diagnostics and therapy monitoring in clinical settings.

5.4. Aptamer-integrated CRISPR biosensor

Aptamers are short, single-stranded nucleic acids that adopt-specific three-dimensional conformations, enabling them to bind with high specificity and affinity to a diverse array of targets, including proteins, small molecules, metal ions, and even whole cells.²⁸⁷ Integrating aptamers with CRISPR-Cas biosensing platforms significantly expands their functionality beyond nucleic acid detection, enabling CRISPR-mediated identification of a broader range of biological targets. Mechanistically, aptamer-CRISPR biosensors operate through a target-induced conformational change in the aptamer.¹⁶⁰ Upon recognizing its ligand (e.g., thrombin or ATP), the aptamer either releases or reveals a trigger DNA or RNA sequence that subsequently activates a CRISPR-Cas system.²⁸⁸ The activated Cas effector then engages in collateral cleavage of reporter molecules, leading to a detectable signal such as fluorescence or an electrochemical readout.²³⁸ One well-documented application involves the aptamer-Cas12a detection of thrombin, a critical biomarker in coagulation and cardiovascular diseases.²⁸⁹ In this system, thrombin binding induces a structural switch in the aptamer, releasing a pre-hybridized DNA strand that activates Cas12a-mediated collateral cleavage.²⁹⁰ This approach has demonstrated attomolar sensitivity in complex biological matrices, including plasma and serum, without the need for nucleic acid amplification.²⁹¹ Recent innovations have expanded this model to dual-target biosensors, such as those detecting both thrombin and ATP, by using orthogonal aptamers and corresponding Cas enzymes.²⁹² These multiplexed systems enable simultaneous monitoring of multiple biomarkers, enhancing diagnostic accuracy in complex diseases such as cancer and sepsis.^{293,294} Furthermore, in infectious disease diagnostics, aptamer-Cas13a platforms have been developed to detect bacterial toxins such as Staphylococcal enterotoxin B.^{295,296} Here, aptamers serve as the

initial biorecognition elements, while the CRISPR component ensures signal amplification and transduction. These systems provide high specificity and reduce cross-reactivity, particularly important in pathogen-rich environments.²⁴⁵ The major advantages of aptamer-CRISPR integration include their exceptional molecular REC specificity, which is comparable to that of antibodies but with greater chemical stability and ease of synthesis.²⁹⁷ Aptamers can be custom-engineered to bind a virtually unlimited range of molecular targets, making the platform highly versatile. Furthermore, aptamer-CRISPR systems are compatible with various signal detection strategies, including colorimetric, fluorescent, electrochemical, and bioluminescent outputs, enabling their application across multiple diagnostic platforms and clinical settings.²⁴⁵ Despite their advantages, challenges such as ensuring aptamer stability in physiological fluids, avoiding non-specific activation of Cas effectors, and scaling production for clinical deployment remain.²⁹⁸ However, advances in Systematic Evolution of Ligands by Exponential Enrichment and aptamer engineering are addressing these limitations. As this synergy continues to evolve, it is likely to fuel breakthroughs in precision diagnostics, real-time monitoring, and even smart theranostic systems for personalized medicine.

5.5. Nanotechnology-enhanced CRISPR biosensors

Nanotechnology-CRISPR platforms integrate the molecular specificity of CRISPR-Cas systems with the unique physicochemical properties of nanomaterials to enhance diagnostic sensitivity, delivery efficiency, and therapeutic precision.²⁹⁹ By leveraging nanocarriers such as AuNPs, liposomes, lipid nanoparticles, graphene oxide, and magnetic beads, researchers have significantly improved the stability, biocompatibility, and cellular targeting of CRISPR-based systems in both *in vitro* diagnostics and *in vivo* applications.³⁰⁰⁻³⁰³ These nanomaterials protect CRISPR components, including Cas proteins and gRNAs, from NUC-mediated degradation while facilitating their cellular uptake, endosomal escape, and nuclear localization.³⁰⁴ For example, an AuNP-based CRISPR delivery system has been developed to repair genetic mutations linked to muscular dystrophy, in which polyethylene glycol-coated nanoparticles deliver gRNA and Cas9 to facilitate cell repair.³⁰⁵ The integration of magnetic nanoparticles with CRISPR has also enhanced the sensitivity and accuracy of biomolecular detection, allowing earlier disease detection and treatment.³⁰⁶ In one platform, magnetic bead-Cas12a complexes were used for the isolation and detection of HPV DNA, improving both the signal-to-noise ratio and reproducibility of detection assays.³⁰⁷ These systems also allow for pre-concentration of low-abundance biomarkers, enabling detection at attomolar levels without amplification. Beyond DNA/RNA detection, nanomaterial-CRISPR constructs have been applied in point-of-care immunodiagnostics, such as multiplexed lateral flow assays using AuNP-Cas conjugates, and even in sono-immunotherapy, where CRISPR-functionalized nanobubbles release their payload in response to ultrasound.³⁰⁸⁻³¹⁰ Furthermore, liposome-based CRISPR delivery vehicles are being optimized for non-invasive administration routes, including nasal and oral formulations,

which are crucial for decentralized healthcare models.³¹¹ This combination of nanotechnology and CRISPR is not only enhancing therapeutic precision and minimizing off-target effects but also expanding the potential of biosensors in real-time, portable, and ultrasensitive diagnostics. As the field advances, nanomaterial-CRISPR hybrids will offer potential for enhancing diagnostic capabilities, increasing treatment precision, and supporting the development of personalized medicine.

5.6. Liquid biopsy biomarkers and CRISPR biosensing

Circulating biomarkers such as cell-free DNA (cfDNA), miRNAs, messenger RNAs, and exosomal RNA have become indispensable tools for non-invasive diagnostics.³¹²⁻³¹⁴ CRISPR-based biosensors have demonstrated significant promise in detecting these biomarkers with high sensitivity and specificity, transforming liquid biopsies into powerful platforms for early disease detection, real-time monitoring, and prognosis.³⁰² One of the key strengths of CRISPR diagnostics is their adaptability to detect low-abundance nucleic acids in blood, plasma, saliva, and urine without the need for complex infrastructure.⁴⁵ Cas12a and Cas13a effectors are particularly suited for this application. Cas12a targets DNA-based markers such as cfDNA fragments from tumors or pathogens, while Cas13a excels at sensing small non-coding RNAs like miRNAs.³¹⁵ In oncology, cfDNA released by tumor cells harbors signature mutations that can be detected using CRISPR-Cas12a systems. These systems are capable of identifying mutations in the *EGFR*, *KRAS*, or *TP53* genes, allowing for earlier cancer detection or monitoring of treatment response.³¹⁶ Cas14-based platforms, with their ability to recognize ssDNA at high resolution, are also emerging as powerful tools for SNV detection in cfDNA.¹⁵² miRNAs, such as miR-21, miR-155, and miR-20a, are well-established circulating markers in cancers and cardiovascular diseases.^{207, 317,318} CRISPR-Cas13a biosensors have demonstrated efficient detection of these miRNAs, benefiting from the enzyme's RNA-guided collateral cleavage activity that amplifies signal output.²⁰⁷ These sensors can even be integrated into lateral flow strips or microfluidic chips for rapid bedside analysis. Exosomal RNAs, including messenger RNAs and miRNAs enclosed within extracellular vesicles, are gaining REC for their diagnostic value in neurological diseases and aggressive tumors.³⁴² Cas13-based biosensors, when combined with vesicle isolation techniques, have shown the ability to detect exosomal RNA cargo with precision, opening avenues for early-stage diagnostics in diseases such as glioblastoma or pancreatic cancer.³¹⁸ Furthermore, CRISPR biosensors are being developed to simultaneously detect multiple biomarkers from a single sample, enabling multiplex diagnostics. For example, triple detection of miR-21, miR-375, and miR-141 can differentiate between subtypes of prostate cancer,³¹⁹ while combined analysis of miR-122 and hepatitis B virus RNA provides insights into liver disease progression.³²⁰ The ability to harness circulating biomarkers using programmable CRISPR tools brings the diagnostic process closer to real-time, patient-friendly testing. It also paves the way for predictive medicine, where disease risk can be assessed long before symptoms appear.

6. Clinical and translational applications

The integration of CRISPR-Cas systems with biosensing technologies has significantly advanced diagnostics, disease monitoring, and molecular medicine. The high specificity of CRISPR effectors in nucleic acid REC, coupled with their programmability and collateral cleavage capabilities, has established them as powerful platforms for next-generation biosensors.⁴² These tools have shown exceptional sensitivity and specificity in detecting nucleic acid targets, biomarkers, and pathogens across various clinical and environmental settings. As illustrated in **Figure 8**, the complete translational pipeline, from molecular design to functional implementation, has matured to support real-world integration in both diagnostic and therapeutic frameworks. Furthermore, since its groundbreaking use in genome editing was demonstrated in 2013, CRISPR/Cas9 has been adapted for diagnostic platforms, enabling the development of portable, cost-effective, and fast detection systems.²⁴² Researchers have integrated Cas enzymes into microfluidic models, paper-based assays, and smartphone-compatible devices, enabling real-time analysis of biological signals even in resource-limited settings. These platforms are capable of identifying targets ranging from emerging viral pathogens to single-nucleotide mutations in oncogenes and rare genetic disorders.²²¹ As research continues to optimize gRNA design, enzyme engineering, and delivery systems, these platforms are becoming more robust and adaptable to complex biological samples.³²¹ In the following sections, we explore the expanding translational landscape of CRISPR diagnostics, covering POC innovations, AI-assisted platforms, emerging theranostic strategies, and broader applications in biotechnology, synthetic biology, and sustainable healthcare.

Recent advancements have explored the integration of CRISPR platforms with other functional nucleic acids, including aptamers, ribozymes, small interfering RNA (siRNAs), and peptide nucleic acids (PNAs), to enhance both diagnostic and therapeutic potential.³²² CRISPR-aptamer hybrids have been employed in biosensing platforms to improve sensitivity and enable rapid, point-of-care detection of disease biomarkers.⁴⁵ Similarly, ribozyme-controlled CRISPR switches provide tunable NUC activation, siRNA co-delivery strategies enhance gene-silencing efficiency, and PNA-assisted CRISPR approaches improve target REC and editing precision.³²³⁻³²⁵ These hybrid systems represent promising next-generation CRISPR-based theranostic tools with improved specificity and clinical applicability.

6.1. Point-of-care CRISPR-Cas technology application

The development of point-of-care kits using CRISPR-Cas systems has been driven by the need for fast, accurate, affordable, and specific diagnostic tools that can be used outside traditional laboratory settings, especially in resource-limited areas.²³⁸ Standard POCT, such as rapid strep tests, glucose monitoring, and pregnancy tests, provide instant results, enabling medical professionals to determine the appropriate treatment quickly.³²⁶ For instance, a rapid strep test can instantly confirm the presence of strep throat, allowing the physician to prescribe the necessary antibiotics.³²⁷ Similarly,

CRISPR-AI theranostics

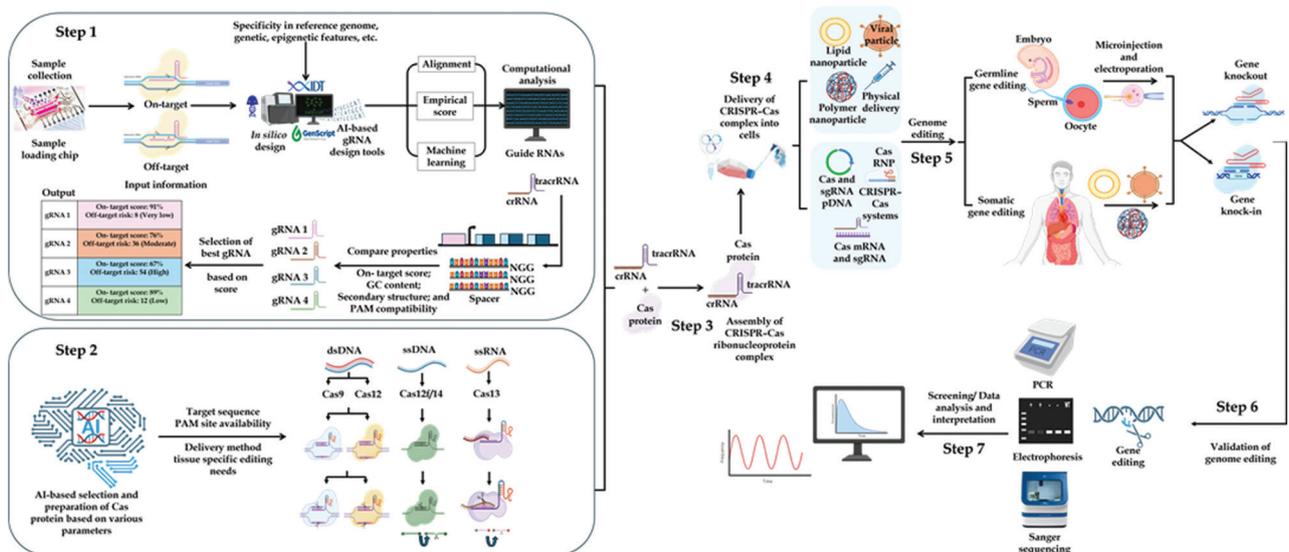


Figure 8. AI-assisted CRISPR–Cas genome editing workflow from sample to validation. This figure presents an AI-integrated CRISPR–Cas workflow, beginning with Step 1, where biological samples are collected, nucleic acids are extracted, and target regions are analyzed using AI-based *in silico* gRNA design tools. Machine learning models evaluate gRNAs based on on-target efficiency, off-target risk, and structural features to identify the most suitable candidates. In Step 2, AI assists in selecting the appropriate Cas variant based on PAM compatibility, target type, and delivery constraints. In Step 3, the selected gRNA and Cas protein are assembled into a CRISPR–Cas RNP complex. In Step 4, the complex is delivered into cells via physical or chemical methods. Step 5 involves genome editing in either germline or somatic cells, resulting in gene knockout or knock-in via NHEJ or HDR pathways. In Step 6, editing outcomes are validated using PCR, electrophoresis, and sequencing techniques. Finally, in Step 7, AI assists in the analysis and interpretation of results, providing feedback to enhance the precision of future editing cycles. Figure created by the authors.

Abbreviations: AI: Artificial intelligence; Cas: CRISPR-associated protein; CRISPR: Clustered regularly interspaced short palindromic repeats; crRNA: CRISPR RNA; dsDNA: Double-stranded DNA; gRNA: Guide RNA; HDR: Homology-directed repair; mRNA: Messenger RNA; NHEJ: Non-homologous end joining; PAM: Protospacer adjacent motif; PCR: Polymerase chain reaction; pDNA: Plasmid DNA; RNP: Ribonucleoprotein; sgRNA: Single guide RNA; ssDNA: Single-stranded DNA; ssRNA: Single-stranded RNA; tracrRNA: Trans-activating CRISPR RNA.

glucose monitoring aids diabetics in managing their blood sugar levels in real time.³²⁸ Key technological advancements, including SHERLOCK in 2017, DETECTR in 2018, and the incorporation of paper-based platforms and lateral flow assays in 2019, have significantly contributed to the development of CRISPR-Cas POC kits as mentioned in **Table 7**.³²⁹ Using lateral flow assays, the first CRISPR-Cas kits for COVID-19 were based on SHERLOCK (Cas13-based RNA detection) and DETECTR (Cas12-based RNA-to-DNA detection), which provided a rapid (30–60 min) and low-cost method to detect SARS-CoV-2.^{330,331}

Diagnostic methods with a lower limit of detection can detect diseases earlier, when the pathogen load is typically low, allowing more accurate and timely medical interventions.³³⁷ The ability of next-generation CRISPR diagnostics to detect multiple targets simultaneously has greatly enhanced their versatility. Advances in smartphone-based devices and handheld fluorescence readers have also increased the portability of these technologies. One notable example is the Streamlined Highlighting of Infections to Navigate Epidemics platform, which combines SHERLOCK and Heating Unextracted Diagnostic Samples to Obliterate NUC technologies to enable real-time viral RNA detection on portable devices.²⁸⁰ Building on this, the Minimally Instrumented SHERLOCK platform developed at MIT enables variant-level detection of SARS-CoV-2 and integrates seamlessly with a smartphone

for real-time readouts, offering rapid, multiplexed, and cost-effective diagnostics in field settings.³³⁸ The advantages of POCT include reduced wait times for patients, especially in emergencies, and the elimination of multiple appointments, which in turn reduces overall healthcare costs.³³⁹ Moreover, POCT enables quicker adjustments to treatment plans, enhancing patient satisfaction and outcomes.

The integration of CRISPR detection with microfluidic platforms has further improved the automation of sample processing and increased test throughput.³⁴⁰ Researchers are also working to optimize these kits for operation at ambient temperatures and to reduce sample preparation steps, such as extraction-free processing, thereby improving on-site usability.^{341–343} These enhancements make CRISPR-Cas point-of-care kits more accessible, effective, and affordable, especially in low-resource environments. CRISPR-based liquid biopsy tests for genetic disorders and cancer biomarkers are becoming feasible, offering high-sensitivity electrochemical CRISPR biosensors that deliver rapid results without requiring expensive sequencing technologies.³⁴⁴ Recent innovations, such as the INSPECTR platform developed by Mammoth Biosciences, demonstrate how synthetic DNA circuits and lyophilized reagents can enable instrument-free, paper-based POC diagnostics.³⁴⁵ In addition, wearable biosensing devices, such as graphene-integrated microneedle patches, now allow real-time monitoring of circulating biomarkers, including

Table 7. CRISPR-Cas systems in point-of-care (POC) diagnostics: Features, applications, and challenges

Feature/system	Description	Cas enzyme(s) used	Readout method	Key advantages for POC	Applications	Limitations/challenges for POC	References
SHERLOCK	(Specific High-sensitivity Enzymatic Reporter unLOCKing) - A foundational CRISPR-Cas POC platform	Cas13 (primarily Cas13a)	Fluorescence (plate reader, handheld fluorimeter, smartphone adapter); LFA	Ultrasensitive (attomolar), highly specific (single-base mismatch), direct RNA detection (no RT needed), multiplexing	RNA viruses (e.g., SARS-CoV-2, Zika, dengue, Lassa, Nipah, HIV), bacterial RNA, and cancer biomarkers (miRNAs)	Requires pre-amplification for ultra-low targets (adds steps). Fluorescence readouts require a device, though increasingly portable. LFA may have lower sensitivity	332
DETECTR	(DNA Endonuclease-Targeted CRISPR Trans Reporter) - Another foundational CRISPR-Cas POC platform	Cas12a (e.g., LbCas12a, AsCas12a)	Fluorescence (plate reader, handheld fluorimeter, smartphone adapter); LFA	High sensitivity (attomolar), highly specific (SNP detection), direct DNA detection, robust, and rapid	DNA virus detection (e.g., HPV, African swine fever virus), bacterial pathogens (e.g., <i>Mycobacterium tuberculosis</i>), and genetic mutations	Requires pre-amplification for low targets. Fluorescence readouts require a device. LFA may have lower sensitivity. Primarily targets dsDNA	232
HOLMES	(One-Hour Low-cost Multipurpose highly Efficient System) - Optimized versions of DETECTR for enhanced performance	Cas12a, Cas12b	Fluorescence, LFA	Improved speed and ease of use, reduced contamination risk with one-pot design, high sensitivity, and specificity	Pathogen detection, including DNA viruses, bacteria, and multiplexed assays	Still in development for widespread adoption. Optimization required for each new target	333
CARMEN	(Combinatorial Arrayed Reactions for Multiplexed Evaluation of Nucleic Acids) - A highly multiplexed platform	Multiple Cas enzymes (e.g., Cas13, Cas12)	Fluorescence imaging (specialized reader)	Extremely high multiplexing capability, comprehensive sample analysis	Pathogen surveillance, pan-viral screening, and complex diagnostic panels	Requires specialized array readers and more complex data analysis. Not a simple "strip" POC test	43
CRISPR-Chip/E-CRISPR	Integrates Cas activity with electrochemical sensing for sensitive and rapid detection	dCas9 (binding), Cas12a, Cas13a (cleavage)	Electrochemical (potentiostat, custom chip readers)	High sensitivity, quantitative potential, rapid readout, potential for miniaturization and automation, direct electrical signal (no optics needed)	Pathogens, cancer biomarkers, and environmental contaminants.	Requires microfabrication for chip development. Still needs further validation in complex real-world samples	334
Cas14-based POC	Utilizes the miniature Cas14 enzyme for direct ssDNA detection	Cas14a	Fluorescence, LFA, colorimetric	Very small size (facilitates miniaturization), PAM-independent for ssDNA targeting (flexible design), high specificity (SNP detection)	ssDNA virus detection (e.g., parvoviruses), genotyping, and specific mutation detection	Requires conversion of dsDNA to ssDNA for many targets. Not as widely studied or commercialized compared to Cas12/13	268
CRISPR-Dx coupled with LFA	General category of CRISPR-Cas systems integrated into LFA formats	Cas12a, Cas13a	Visual (colorimetric band on a strip)	Extremely simple, low-cost, equipment-free, rapid (minutes), suitable for field use and resource-limited settings	Infectious diseases (e.g., COVID-19, influenza, tuberculosis, malaria), agricultural diagnostics, and food safety	Lower sensitivity compared to fluorescence-based methods, typically qualitative or semi-quantitative. Risk of false positives if not handled carefully (e.g., contamination)	335
CRISPR-Dx coupled with isothermal amplification	All CRISPR-Cas POC systems often rely on a pre-amplification step to boost sensitivity	Cas9, Cas12, Cas13, Cas14	Fluorescence, LFA, colorimetric, electrochemical	Eliminates the need for thermal cyclers (like PCR), enabling truly portable and battery-operated devices. Achieves extremely high sensitivity	Risk of contamination if not designed as a "one-pot" system	Essential for ultrasensitive detection in most real-world scenarios	336

Abbreviations: AsCas12a: *Acidaminococcus* Cas12a; CRISPR-Cas: Clustered regularly interspaced short palindromic repeats and CRISPR-associated protein; CRISPR-Dx: CRISPR-based diagnostics; dCas9: Catalytically inactivated Cas9; dsDNA: Double-stranded DNA; E-CRISPR: CRISPR-Cas12a (gpf1)-based electrochemical biosensor; HPV: Human papillomavirus; LbCas12a: *Lachnospiraceae* bacterium Cas12a; LFA: Lateral flow assay; miRNA: MicroRNA; PAM: Protospacer adjacent motif; PCR: Polymerase chain reaction; RT: Reverse transcription; SNP: Single-nucleotide polymorphism; ssDNA: Single-stranded DNA.

cfDNA. For instance, a CRISPR-Cas9 microneedle patch integrating graphene biointerfaces enabled *in vivo* monitoring of cfDNA in interstitial fluid with femtomolar sensitivity over 10 days in mice.³⁴⁶

Future updates include the discovery of smaller CRISPR proteins like Cas14, which targets ssDNA, to facilitate the development of miniaturized diagnostic platforms.²²⁶ Digital platforms, including cloud data sharing, AI-driven analysis, and smartphone-based detection, are being integrated into CRISPR diagnostics to enable point-of-care kits to deliver real-time data analysis and support epidemiological tracking.³⁴⁷ The integration of CRISPR-based biosensors into wearable devices allows real-time monitoring of disease biomarkers, opening new avenues for personalized medicine. With high accuracy and efficiency, CRISPR-Cas could transform diagnostic medicine and streamline treatment decisions.³⁴⁸ Ongoing research and investment are essential to fully harness their potential in POCT applications.

6.2. AI-augmented CRISPR diagnostics

While CRISPR-based genetic medicine has shown great promise, its clinical use is still limited by challenges such as off-target effects, delivery inefficiencies, limited control over editing outcomes, and variability in patient responses. These challenges emphasize the need for smarter, adaptive systems that can improve both the accuracy and safety of genome editing. Building on the foundation of CRISPR-based genome editing, the integration of AI is now accelerating the development of precision and personalized medicine. The combination of AI and CRISPR-Cas biosensing is ushering in a new era of diagnostics that are more intelligent, faster, and more predictive.⁴⁵ While CRISPR provides the molecular precision required to detect specific nucleic acid targets, AI enhances the interpretation, accuracy, and adaptability of these diagnostic platforms, especially in high-throughput or point-of-care settings. One of the earliest and most important applications of AI in CRISPR diagnostics is in gRNA design. Beyond gRNA optimization, AI plays a crucial role throughout the entire CRISPR diagnostic workflow, from image interpretation in

biosensors to the prediction of editing outcomes.³⁴⁹

Deep learning models such as convolutional neural networks (CNNs) and recurrent neural networks are employed to interpret complex fluorescence or electrochemical patterns generated by CRISPR-based biosensors.^{350,351} For instance, CNN architectures trained on labeled fluorescence images from SHERLOCK assays enable real-time signal interpretation and noise discrimination in smartphone-integrated diagnostic platforms.³⁵² In addition, sequence-based prediction models, such as DeepCRISPR, utilize high-throughput datasets such as genome-wide, unbiased identification of DSBs enabled by sequencing (GUIDE-seq) to train deep neural networks for accurate on- and off-target cleavage prediction.⁶⁷ These models incorporate parameters such as chromatin accessibility, PAM proximity, and nucleotide content, resulting in improved precision over traditional heuristics. Such integrative methods enable context-aware gRNA optimization, enhancing editing efficiency across various genomic contexts. For instance, models such as DeepSpCas9 and DeePHF include chromatin state and thermodynamic stability to predict cell-type-specific gRNA performance, addressing differences between primary tissues and immortalized cell lines.^{353,354}

Moreover, AI-assisted models are being adapted for CRISPRa/i applications, where predicting binding affinity and transcriptional impact is more complex than assessing cleavage efficiency. For example, in 2022, Xu *et al.*¹⁴ developed MiCaR, a microfluidic CRISPR-Cas12a platform capable of multiplex detection of up to 30 viral targets (e.g., nine HPV subtypes and eight respiratory viruses) within 40 min, achieving ~0.26 attomole sensitivity with 97.8% accuracy. These advances underscore how AI integration enhances signal deconvolution and multiplex accuracy, complementing CRISPR's detection capabilities for field-ready diagnostics. These tools are particularly valuable for the development of multiplexed diagnostics and therapeutic strategies, where off-target effects, guide competition, and signal interference must be minimized through precision modeling.³⁵⁵ **Table 8** summarizes the integration of AI across various CRISPR-Cas systems in gene editing, diagnostics, and therapeutic workflows. As these AI platforms continue to mature, their integration into closed-loop diagnostic-therapeutic systems is

Table 8. CRISPR-Cas systems and their applications in medical genetics, enhanced by artificial intelligence

CRISPR-Cas system type	Key features	Applications in medical genetics	How AI enhances applications	References
CRISPR-Cas9	Most widely studied and utilized; uses a single guide RNA (sgRNA) and the Cas9 enzyme	Gene editing, therapies for inherited diseases and cancer, disease modeling	Predicts optimal sgRNAs, classifies variants, and aids in therapy design	356
CRISPR-Cas12 (e.g., Cas12a/Cpf1)	Smaller than Cas9; cleaves DNA with staggered ends; exhibits collateral ssDNA cleavage activity	Diagnostics for pathogens, cancer, and mutations; supports multiplex detection	Analyzes signals, detects diagnostic patterns, and enables point-of-care applications	357
CRISPR-Cas13 (e.g., Cas13a)	Targets and cleaves RNA; exhibits collateral RNA cleavage activity	RNA virus detection, biomarker analysis, RNA editing	Optimizes RNA target selection and tracks expression changes	358
Base editing (e.g., ABEs, CBEs)	Employs a Cas protein (often dead Cas9) fused with a deaminase enzyme to change a single nucleotide	Precise correction of point mutations with minimal off-targets	Predicts off-targets and optimizes base editor design	359
Prime editing	Uses a reverse transcriptase fused to a Cas protein to directly insert or modify DNA sequences	Corrects a broad range of mutations with high accuracy; suitable for complex disorders	Assists in designing prime editors, improves prediction of editing outcomes, and enhances accuracy for complex genetic disorders	360

Abbreviations: ABEs: Adenine base editors; CBEs: Cytosine base editors; CRISPR-Cas: Clustered regularly interspaced short palindromic repeats and CRISPR-associated protein.

expected to reduce the experimental burden, streamline clinical validation, and support adaptive CRISPR workflows in real-world patient settings. **Figure 8** offers a step-by-step overview of the AI-assisted CRISPR-Cas editing workflow, illustrating how AI models predict and rank gRNA candidates based on specificity, off-target risk, and structural suitability. This is followed by the formation, delivery, and editing outcomes of the RNP complex in both germline and somatic contexts. As shown in **Figure 8**, advanced AI-driven platforms extend beyond initial gRNA screening by incorporating large-scale genomic datasets to enhance gRNA performance predictions, taking into account thermodynamic stability, structural compatibility, chromatin accessibility, and sequence context. These improved designs enhance both sensitivity and on-target accuracy while reducing unintended effects across diverse genomic landscapes.²² To achieve this, ML models are trained using labeled datasets such as GUIDE-seq and circularization for *in vitro* reporting of cleavage effects by sequencing (CIRCLE-seq), incorporating sequence motifs, secondary structures, and thermodynamic profiles to predict gRNA efficiency and specificity. These models consistently outperform traditional rule-based algorithms and enable the generation of highly optimized guides for both research and clinical applications.³⁵⁴

AI is also playing a crucial role in signal interpretation and noise reduction in CRISPR-based biosensors. For fluorescence-based and lateral flow platforms, CNNs and computer vision tools can differentiate true positive signals from background noise, thereby enhancing diagnostic confidence.³⁶¹ This is particularly useful for smartphone-integrated biosensors, where variations in lighting and environmental conditions can impact signal accuracy. In multiplexed biosensing setups, where multiple biomarkers are detected simultaneously using a single CRISPR platform, AI is employed to deconvolute complex signal patterns and correlate them with disease states. Moreover, AI is facilitating real-time disease forecasting and adaptive testing strategies.

By integrating CRISPR diagnostic data with patient history, wearable sensor data, or environmental exposure metrics, AI models can predict disease onset, recommend follow-up tests, or dynamically tailor biomarker panels.³⁶² This real-time feedback loop is particularly valuable in managing epidemics or monitoring chronic diseases. Another promising frontier is the application of AI to design synthetic circuits in CRISPR-Dx. These bio-computational systems can execute logical functions (AND, OR, NOT) at the molecular level, enabling CRISPR biosensors to make autonomous decisions, such as releasing a therapeutic payload only when multiple disease markers are detected.^{363,364}

These advances, however, raise important ethical concerns. The use of AI to interpret molecular diagnostics, particularly those involving patient-specific genomic data, necessitates robust safeguards to ensure privacy, data security, and informed consent.³⁶⁵ Furthermore, the explainability of AI models becomes critical in a clinical context; patients and physicians must understand how diagnostic decisions are made, especially when these inform irreversible gene-editing actions.³⁶⁶ Regulatory bodies increasingly recommend the incorporation of transparent AI pipelines and human-in-the-loop designs to mitigate algorithmic bias and ensure accountable decision-making in CRISPR-Dx.³⁶⁷ Overall, AI not only boosts the diagnostic capabilities of CRISPR systems but also makes them more scalable, personalized, and adaptable to emerging clinical needs. The integration of AI across diagnostic, therapeutic, and prognostic domains has progressed to clinical trial stages, encompassing a broad spectrum of diseases and technologies. The future of CRISPR diagnostics lies at the intersection of molecular biology and computational intelligence. Recent breakthroughs have resulted in the development of innovative CRISPR-based biosensing platforms, ranging from wearable and implantable devices to AI-enabled diagnostics, as illustrated in **Figure 9**.

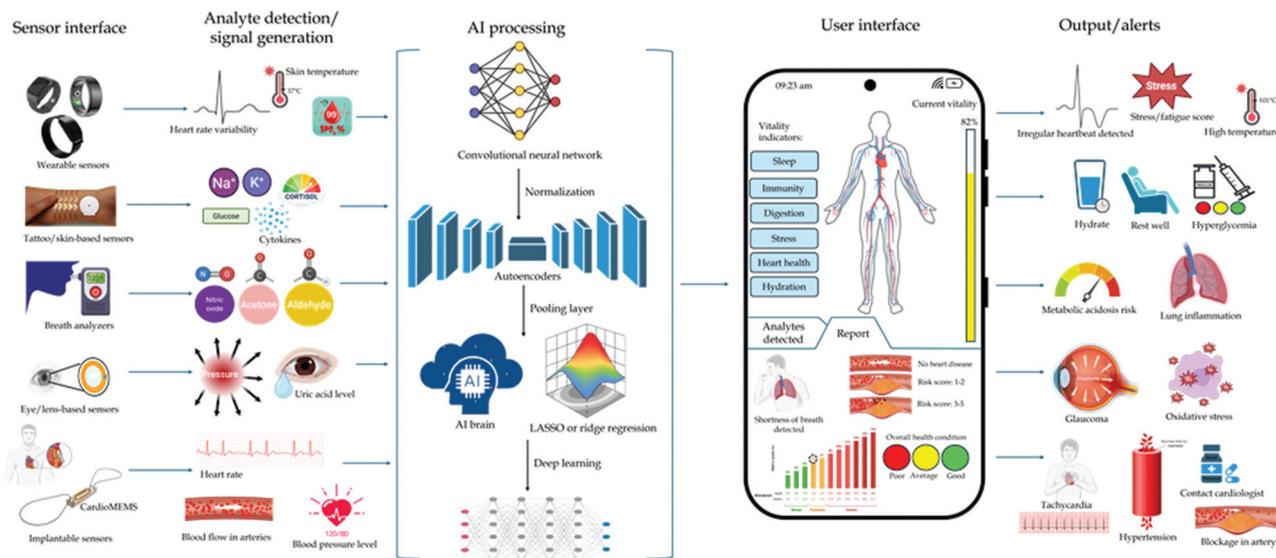


Figure 9. Next-generation biosensors. The figure depicts various innovative wearable, implantable, and biochemical biosensors enabling continuous, non-invasive monitoring of vital health parameters. Figure created by the authors.

Abbreviations: AI: Artificial intelligence; LASSO: Least Absolute Shrinkage and Selection Operator; K⁺: Potassium ion; Na⁺: Sodium ion.

6.3. Theranostic applications - The CRISPR loop

The fusion of diagnostics and therapeutics, known as theranostics, represents one of the most innovative and disruptive applications of CRISPR-Cas systems. This “CRISPR loop” closes the cycle between disease detection and personalized treatment using a single platform to identify a molecular signature and act on it, marking a shift toward precision and autonomous medicine.³⁶⁸ In this approach, a CRISPR-based theranostic framework typically comprises three interconnected functional layers: a biosensor module (e.g., Cas12 or Cas13) that detects disease-specific biomarkers; a decision layer, often augmented by AI for signal interpretation and response modeling; and an effector layer that executes therapeutic interventions through gene editing or transcriptional regulation.³⁶⁹⁻³⁷⁰

Mechanistically, the loop begins with CRISPR-based biosensors identifying molecular anomalies—genetic, epigenetic, or transcriptomic—in patient samples. Once a target is validated, the system either directly activates a therapeutic CRISPR response or sequentially initiates downstream interventions using programmable Cas effectors, executing an autonomous sensing-response cycle, as exemplified by platforms like InCasApt.³⁶³ This closed-loop design enables real-time diagnostics and on-demand therapeutic delivery, pushing the boundaries of personalized medicine. The interplay between CRISPR and AI across each stage of the diagnostic workflow is illustrated in **Table 9**, which outlines how this innovation loop transforms precision diagnostics through continuous feedback, optimization, and automation.

In sickle cell disease, CRISPR-Cas9 has already been used therapeutically to edit the *BCL11A* enhancer and restore fetal

hemoglobin expression. In a theranostic scenario, a CRISPR biosensor could first detect elevated levels of sickling-related biomarkers (e.g., circulating miRNAs or fetal hemoglobin transcript levels) and, upon validation, trigger Cas9-based genome editing.⁴¹⁷ In cancer theranostics, CRISPR-based biosensors can detect circulating tumor DNA mutations, such as those in *TP53*, *KRAS*, or *EGFR*, in blood.³⁷⁵⁻³⁷⁷ Once a mutation is verified, CRISPR effectors, loaded into nanoparticles, viral vectors, or lipid carriers, can be delivered to tumor sites for gene knockout or repair.³⁷⁸ Several preclinical models using Cas9 and Cas12a for such “edit-on-detect” protocols have demonstrated promising results. CRISPR-dCas systems fused to transcriptional regulators (CRISPRa/CRISPRi) are also being investigated for therapeutic gene modulation following the detection of abnormal gene expression.³⁷⁹ For example, Lee *et al.*³⁸⁰ successfully used dCas9-VPR delivered through peptide-imprinted nanoparticles to induce insulin production in glucose-stimulated HEK293T cells, highlighting the potential of this approach for diabetes management.

To improve specificity and prevent premature activation, researchers are developing logic-gated CRISPR systems that activate only when multiple disease-specific inputs are present, such as a combination of RNA biomarkers and protein markers.³⁸¹ This adds a safety buffer, ensuring that editing or silencing is triggered only under pathophysiologically relevant conditions. Some platforms, like CRISPR recorders, are being explored to log cellular events over time, providing a molecular timeline that could enhance personalized treatment response strategies.³⁸² Theranostic CRISPR loops also enable longitudinal health monitoring, where repeated sampling and molecular feedback allow the system to modify therapeutic

Table 9. CRISPR-Cas artificial intelligence (AI) in diagnostics: The innovation loop

Stage in the loop	CRISPR-Cas role	AI's role	Impact on medical genetics diagnostics	References
1. Target identification and discovery	CRISPR-Cas systems (e.g., Cas9, Cas12, Cas13) detect disease-related DNA/RNA sequences	Identifies key biomarkers and CRISPR targets from omics data	Accelerates the discovery of novel diagnostic targets for inherited diseases, infectious agents, and cancer, making diagnostics more comprehensive and precise	371-373
2. Assay design and optimization	Selects appropriate Cas types and designs guide RNAs for specific targets	Predicts optimal gRNAs and assay conditions to minimize off-targets	Reduces experimental trial-and-error, accelerating the development of highly accurate and reliable diagnostic tests. Improves the robustness and performance of CRISPR-based assays	
3. Diagnostic platform development	Integrates CRISPR into formats such as strips, chips, or portable devices	Designs POC-friendly, automated, and efficient platforms	Enables the development of rapid, portable, and cost-effective diagnostic tools suitable for diverse settings, from clinics to remote areas. Reduces reliance on centralized laboratories	
4. Data acquisition and processing	Generates raw detection signals (e.g., fluorescence, sequencing data)	Processes and extracts meaningful signals from assay outputs	Ensures high-quality data input for accurate diagnosis, even with complex or low-concentration samples. Speeds up data interpretation and minimizes human error	
5. Interpretation and reporting	Indicates the presence of genetic markers via cleavage or activation events	Generates specific, detectable readouts (e.g., fluorescence or colorimetric signals) that reflect underlying genetic variations	Delivers faster, more accurate, and nuanced diagnostic reports. Moves beyond simple binary outcomes (positive/negative) to provide deeper insights into patient health and disease prognosis. Facilitates personalized medicine	
6. Feedback and refinement	Uses real-world performance data to improve assay design	Learns from outcomes to refine target selection and optimize assay protocols	Drives continuous improvements in diagnostic accuracy, sensitivity, and efficiency. Supports adaptive learning, making the diagnostic systems more robust and responsive to new genetic variants and disease challenges	

Abbreviations: CRISPR-Cas: Clustered regularly interspaced short palindromic repeats and CRISPR-associated protein; gRNAs: Guide RNAs; POC: Point-of-care.

strategies adaptively. This holds promise for diseases with dynamic molecular signatures, such as cancer, autoimmune disorders, and neurodegenerative diseases.³⁶⁸ Clinically, theranostic approaches have already begun transforming disease management pathways. For example, in prostate cancer, prostate-specific membrane antigen (PSMA)-based radiotheranostics enable simultaneous diagnosis using ⁶⁸Ga-labeled tracers and therapy with ¹⁷⁷Lu-PSMA.³⁸³

In infectious diseases, CRISPR-Cas diagnostic platforms such as SHERLOCK have been coupled with programmable drug delivery systems to simultaneously detect and suppress viral infections.³⁸⁴ In glioblastoma, magnetic resonance imaging-visible nanoparticles loaded with redox-activated therapeutic agents have demonstrated real-time imaging and localized treatment in preclinical models, exemplifying the potential of fully integrated diagnostic-therapeutic systems.³⁸⁵ From a regulatory perspective, the dual-function nature of CRISPR-based theranostic platforms introduces unique challenges. Unlike traditional diagnostics or therapies, these systems operate as integrated, closed-loop architectures, often utilizing AI algorithms that interpret biosensor data and autonomously direct genetic interventions. Therefore, they must simultaneously comply with regulatory standards for *in vitro* diagnostics, such as the Clinical Laboratory Improvement Amendments.³⁸⁶ Existing regulatory pathways are being challenged by the novelty of AI-guided, dynamically adapting gene-editing systems, prompting the development of new paradigms that consider software as a medical device, algorithm versioning, and continuous learning models.³⁸⁷ Regulatory convergence on these hybrid platforms will be vital for their safe clinical deployment. Overall, these advances highlight the transformative potential of AI-integrated CRISPR theranostics in delivering adaptable, autonomous, and highly personalized healthcare solutions.

6.4. Beyond medicine

CRISPR-Cas technology, initially recognized for its transformative impact on genetic diagnostics and therapeutics, has also emerged as a powerful tool in non-medical sectors such as industrial biotechnology, synthetic biology, agriculture, and environmental management.³⁸⁸ In healthcare, CRISPR has been deployed in clinical trials for treating monogenic diseases such as sickle cell anemia and β -thalassemia, where it facilitates the correction of disease-causing mutations by targeting the *BCL11A* enhancer to restore fetal hemoglobin expression.^{389,390} The platform is also being used to develop next-generation immunotherapies, including CRISPR-edited chimeric antigen receptor T-cell (CAR-T) cells for improved cancer targeting, editing of oncogenes for tumor suppression, and immune system modulation for chronic infections.³⁹¹

In agriculture, CRISPR is utilized to boost crop yields, improve disease resistance, and develop plants that can withstand harsh environmental conditions.³⁹² For instance, CRISPR has been applied to generate disease-resistant rice varieties, drought-tolerant maize, and non-browning mushrooms, offering more resilient and sustainable food systems. Livestock breeding programs are also adopting CRISPR to accelerate

the development of disease-resistant or high-productivity animal strains, thereby improving food security and economic efficiency.³⁹³ CRISPR-Cas systems are instrumental in industrial biotechnology, enabling the production of biofuels, bioplastics, and high-value biopharmaceuticals such as insulin, vaccines, and antibiotics in engineered microbial hosts with enhanced yields and reduced production costs.^{394,395} Synthetic biology applications utilize CRISPR for genome-scale engineering, metabolic pathway optimization, and microbial strain development. In basic and translational research, CRISPR enables high-throughput functional genomics through knockout and activation screens, accelerating the identification of genes involved in drug response, tumor progression, and disease resistance.³⁹⁶⁻³⁹⁹ Furthermore, epigenome editing with catalytically deactivated Cas proteins (dCas9/dCas12), fused to transcriptional regulators, allows for precise gene expression modulation without altering the underlying DNA sequence—a promising avenue for studying complex disorders such as autism, Alzheimer's disease, and depression.^{400,401} CRISPR's potential also extends to environmental conservation and sustainability. Gene drives based on CRISPR-Cas9 are being designed to control invasive species, suppress disease-transmitting mosquito populations, and preserve biodiversity.⁴⁰² In microbial ecology, CRISPR tools help monitor and engineer microbiomes for soil remediation, wastewater treatment, and greenhouse gas mitigation.⁴⁰³⁻⁴⁰⁴ Overall, the expansion of CRISPR-Cas technology into agriculture, industrial biotech, and environmental applications showcases its versatility and transformative potential across multiple sectors, offering robust solutions for global challenges ranging from food security to climate change.

7. Limitations and translational challenges

Despite rapid advances in CRISPR-based biosensing and therapeutics, several technical, biological, regulatory, and ethical challenges continue to limit their broad clinical implementation. Translating these systems from the laboratory to real-world healthcare environments requires not only solving scientific limitations but also addressing practical, societal, and governance-related concerns. A major technical limitation lies in off-target activity, especially in Cas9- and Cas13-based systems. Although various CRISPR-Dx rely on collateral cleavage, non-specific activation due to poor gRNA design or suboptimal assay conditions can lead to false positives or background noise.^{406,407} Enhanced gRNA design algorithms and the development of high-fidelity Cas variants, particularly in Cas9 systems, are critical to improving specificity.⁴⁰⁸ In addition, sample preparation remains a bottleneck, as many biosensors require high-purity nucleic acids, which are difficult to isolate from complex biofluids like saliva or plasma, particularly in low-resource settings.^{409,410} This challenge necessitates innovations in extraction-free, direct-detection strategies and inhibitor-resistant assay chemistries. Field-deployable diagnostics are further constrained by the temperature sensitivity of reagents and reliance on isothermal amplification methods such as RPA and LAMP, which typically require cold chain storage and precise thermal conditions.²⁷⁷ To overcome this, researchers are engineering thermostable

Cas proteins and lyophilized assay formulations that retain functionality at ambient temperatures.⁴¹¹

Multiplexing, while promising, introduces complications such as cross-reactivity and overlapping signal interference. Advanced signal encoding strategies, including fluorescent barcoding and AI-assisted signal deconvolution, offer potential solutions; however, their clinical validation remains limited.⁴¹² Scalability presents another challenge. Manufacturing CRISPR-based biosensors at consistent quality levels demands strict standardization in assay design, production, and validation. Variability in reagents or device assembly can impede regulatory approval processes from authorities such as the United States Food and Drug Administration (FDA) or the European Medicines Agency.¹⁷³ Beyond technical issues, ethical, legal, and social implications are gaining prominence. CRISPR biosensors, especially wearable or autonomous formats, raise concerns about privacy, informed consent, biosurveillance, and data ownership.⁴¹³ Moreover, AI-integrated CRISPR systems bring new challenges regarding algorithmic transparency, patient comprehension, and responsibility in decision-making.⁴¹⁴ From a technical standpoint, AI-driven CRISPR platforms face significant bottlenecks beyond ethical concerns. Biological datasets often suffer from noise, batch effects, and limited sample diversity, which hinder robust model training and reproducibility.⁴¹⁵ Furthermore, models trained on one cell type, species, or assay condition frequently fail to generalize across contexts, limiting translational potential.⁴¹⁶ Recent approaches such as transfer learning, ensemble modeling, and multimodal data integration (e.g., combining genomic, transcriptomic, and imaging datasets) are being explored to mitigate these limitations [³⁵⁶]. However, widespread clinical adoption will require extensive benchmarking across heterogeneous datasets and rigorous external validation. Regulatory agencies and clinical institutions must co-develop transparent, human-in-the-loop frameworks that ensure accountability while promoting innovation.⁴¹⁷ As these platforms become more embedded in everyday health infrastructure, the need for strong global ethical guardrails and cooperative policy frameworks becomes increasingly urgent. Policies must safeguard patient autonomy, guarantee transparent data governance, and promote equitable access, especially in underserved communities.⁴¹⁸ Inclusive design involving patients, clinicians, ethicists, and regulators is essential to avoid reinforcing health inequities. In parallel, international collaboration is necessary to align cross-border standards, ensuring safe and ethical use of CRISPR technologies globally. This includes harmonizing data privacy laws, clinical trial protocols, and equitable access models.⁴¹⁹ Such collaboration could facilitate a unified approach to managing both the risks and rewards of CRISPR-based interventions. Furthermore, theranostic applications, which integrate diagnostics and therapeutics in a single closed-loop system, present regulatory and safety complexities. Current frameworks are ill-equipped to evaluate dual-function platforms, especially those guided by AI.⁴²⁰ As such, there is a pressing need for new regulatory paradigms that accommodate these hybrid technologies. These should address not only efficacy and safety, but also software updates, adaptive algorithms, and ethical deployment.

Finally, practical limitations such as cost, manufacturing complexity, and the potential immunogenicity of bacterial Cas proteins must be addressed to ensure global access and patient safety.^{421,422} Emerging tools, such as logic-gated Cas circuits and CRISPR recorders, offer dynamic control and molecular memory capabilities but face hurdles in biocompatibility, stability, and *in vivo* delivery.⁴²³ In summary, while CRISPR biosensors and theranostics offer unprecedented potential for real-time, personalized, and decentralized medicine, achieving safe and equitable implementation requires overcoming a multilayered set of technical, ethical, and policy-related challenges. A concerted global effort, rooted in responsible innovation and cooperative governance, will be key to unlocking the full translational promise of CRISPR technologies.

8. Precision personalized medicine with CRISPR-Cas: Current impact and future horizons

Having outlined the mechanistic basis and diagnostic applications, it is important to consider how CRISPR may evolve in clinical and translational contexts. CRISPR-Cas technology is rapidly redefining personalized medicine by enabling precision-level interventions tailored to an individual's unique molecular and genetic makeup. The ability to detect, modulate, or correct disease-driving genomic alterations at their origin aligns CRISPR with the core tenets of precision healthcare. Clinical applications are no longer speculative, with real-world therapies emerging across oncology, hematology, infectious diseases, and rare genetic disorders. Notably, CRISPR-Cas9-based gene editing therapies for β -thalassemia and sickle cell disease have entered advanced clinical stages, with FDA-approved treatments like Exagamglogene Autotemcel (developed by CRISPR Therapeutics and Vertex) already marking the transition from bench to bedside. Beyond monogenic disorders, CRISPR's integration with CAR-T therapy has further amplified its translational scope. Engineered immune cells, modified via CRISPR to enhance tumor specificity or evade immune checkpoints, are now being deployed in leukemia and lymphoma trials. Likewise, CRISPR-based human leukocyte antigen (HLA) editing is helping to overcome histocompatibility barriers in allogeneic transplantation, bringing "off-the-shelf" immunotherapies closer to reality. In the realm of diagnostics, HLA genotyping using CRISPR-Cas systems is improving organ transplant matching and autoimmune disease stratification. These innovations are increasingly supported by AI, which enhances gRNA design, predicts off-target edits, and optimizes dosing strategies, driving a convergence of gene editing and computational biology. The growing momentum is also reflected in the economic landscape. According to Precedence Research, the global CRISPR gene editing market was valued at United States dollars (USD) 3.5 billion in 2023 and is projected to surpass USD 15.8 billion by 2032, growing at a compound annual growth rate of 18.5%. This surge is fueled by increasing clinical trials, rising demand for personalized therapies, and expanding applications in diagnostics, agriculture, and synthetic biology (<https://www.precedenceresearch.com/>

crispr-based-gene-editing-market). **Table 10** provides a historical overview of key capital investments and market developments that have shaped the CRISPR-Cas trajectory, highlighting the shift from fundamental discovery to FDA-approved therapies and commercial growth.

Several biotech firms, including CRISPR Therapeutics,⁴⁴¹ Editas Medicine,⁴⁴² Beam Therapeutics,⁴⁴³ Intellia Therapeutics,⁴⁴⁴ and Mammoth Biosciences, are now spearheading CRISPR innovations, with multiple candidates in preclinical and clinical pipelines. However, barriers remain, such as variability in patient responses, challenges in delivery (particularly to immune-privileged tissues like the brain), high treatment costs, and regulatory complexity, all of which must be addressed to ensure equitable access and safety. And therefore, public-private partnerships and government-backed subsidies will be vital in democratizing CRISPR-based personalized medicine. This convergence of molecular biology, computational tools, and patient-centered design is poised to catalyze a paradigm shift from reactive treatments to predictive, preventive, and adaptive interventions. Building on this foundation, the following

subsections explore what CRISPR biosensing may look like by 2030 and how the diagnostic-therapeutic continuum is evolving through smart, scalable platforms.

8.1. CRISPR-integrated wearable biosensors

Miniaturization and hardware integration are likely to redefine how and where CRISPR biosensors are utilized. Wearable devices, such as smartwatches, clothing fabrics, or subdermal chips, embedded with CRISPR detection modules could continuously track biomarkers in sweat, saliva, or interstitial fluid, enabling non-invasive, real-time health monitoring.⁴²¹ For instance, smart patches may detect inflammatory cytokines and activate CRISPR-dCas circuits to suppress harmful gene expression, offering preventive modulation in chronic conditions. These personalized health dashboards, dynamically adjusting to each individual's physiological and genetic signals, represent a paradigm shift toward autonomous, precision-guided healthcare—revolutionizing preventive medicine by enabling early disease detection, timely intervention, and improved quality of life.

Table 10. CRISPR-Cas: Market capital investment trajectory (approximately 2012–2025)

Period	Key developments and investment landscape	Estimated market size/investment highlights (approximate)	References
2005–2011	Discovery and fundamental research phase: CRISPR-Cas was known as a bacterial immune system. Investment was primarily through academic grants and basic science research. No significant “market capital investment” in the commercial sense	Minimal commercial market; focus on basic scientific funding	424
2012–2014	CRISPR-Cas9 gene editing revolution: Key publications (Doudna/Charpentier, Zhang, Church) demonstrate CRISPR-Cas9's ability to edit mammalian cells, sparking intense commercial interest. Formation of early-stage biotech companies	Early VC funding: Millions of dollars in seed and Series A funding for foundational CRISPR companies such as Editas Medicine, CRISPR Therapeutics, and Intellia Therapeutics. For example, Editas Medicine received significant early investment	425-428
2015–2016	“CRISPR hype” and initial public offerings (IPOs): Major pharmaceutical partnerships and IPOs of leading CRISPR companies. Patent disputes began	IPO launches: Editas Medicine and CRISPR Therapeutics went public in 2016, raising hundreds of millions. Intellia Therapeutics also went public around this time. Strategic partnerships: Large pharma companies (e.g., Vertex, Bayer, Novartis, AstraZeneca) initiate collaborations worth hundreds of millions to billions. Example: Vertex-CRISPR Therapeutics deal valued up to \$2.6 billion (2015)	429-432
2017–2019	Clinical trials and pipeline expansion: Lead candidates advanced into clinical trials for genetic disorders (e.g., sickle cell disease, β -thalassemia, eye diseases). Continued VC funding for new entrants and platform technologies	Continued VC and public offerings: Hundreds of millions to billions of dollars raised through additional funding rounds and follow-on public offerings by existing companies. Investor interest in gene editing continued to broaden during this period	433-435
2020	Nobel Prize recognition: Emmanuelle Charpentier and Jennifer Doudna were awarded the Nobel Prize in Chemistry for CRISPR, further legitimizing the field and boosting investor confidence	Increased investment and valuations: Renewed investor interest, often accompanied by higher valuations for CRISPR companies following the Nobel Prize recognition	436,437
2021–2023	Acceleration of clinical progress and first approval: Positive clinical trial data across indications. In December 2023, Casgevy (Vertex/CRISPR Therapeutics) became the first CRISPR-based therapy approved in the UK and US for sickle cell disease and β -thalassemia	Market size growth: The Global CRISPR market is valued at approximately US\$3.2–US\$3.3 billion in 2023 (various sources). Significant late-stage private rounds and public market investments	438,439
2024–2025 (current and near-future)	Post-approval momentum and diversification: Rollout of Casgevy. Ongoing progress in base editing and prime editing. Broader applications in agriculture, diagnostics, and other therapeutic areas gaining traction	Projected global CRISPR market: ~US\$4.0–US\$5.5 billion in 2024–2025 (various reports, including <i>CRISPR and Cas Gene Market</i> , <i>CRISPR-Based Gene Editing Market</i>). Continued investment in new technologies and expanded clinical pipelines	440
Beyond 2025 (forecast)	Sustained high growth: Strong CAGR (11–22% annually) projected, driven by emerging therapies, expanded applications, and improved delivery methods	Forecasted market size: US\$10–US\$17 billion by 2030–2034, indicating substantial future capital investment	439

Abbreviations: CAGR: Compound annual growth rate; CRISPR-Cas: Clustered regularly interspaced short palindromic repeats and CRISPR-associated protein; UK: United Kingdom; US: United States; VC: Venture capital.

8.2. CRISPR-based liquid biopsy platforms

Liquid biopsies provide a minimally invasive approach for monitoring circulating tumor DNA, miRNAs, and exosomes in patient biofluids.⁴⁴⁵ CRISPR-powered assays enhance sensitivity and specificity, supporting early cancer detection, therapy response monitoring, and relapse prediction.⁴⁴⁶ When combined with AI-driven analytics, CRISPR-based liquid biopsies hold strong potential for precision oncology and real-time clinical decision-making.⁴⁹⁴¹ ML algorithms can integrate multi-omic profiles (genomic, transcriptomic, and proteomic data) with CRISPR assay outputs, enabling patient stratification, therapy outcome prediction, and adaptive treatment decisions in oncology and other complex diseases.⁴⁴⁷ Importantly, AI can also reduce noise in CRISPR signal readouts, minimizing false positives while identifying clinically relevant rare events with high accuracy.⁴⁴⁸ Together, the integration of CRISPR diagnostics and AI-driven liquid biopsy analysis holds strong potential for next-generation precision oncology, enabling early detection and more personalized clinical treatments.

While this review emphasizes wearable biosensors and liquid biopsy platforms as particularly promising directions, it is important to note that other innovations, such as synthetic biology-driven gene circuits, advanced multiplexing strategies, and low-cost paper-based diagnostics, also hold significant potential. Together, these complementary approaches ensure that CRISPR technologies continue to advance toward a more accessible, intelligent, and globally equitable future for precision medicine.

9. Conclusions

AI-enhanced CRISPR technology holds great promise for future therapeutic advances. By promoting ethical research practices, fostering interdisciplinary collaboration, and establishing strong regulatory frameworks, the scientific community can ensure that the benefits of AI-enhanced CRISPR are fully and fairly realized. AI is being utilized in digital pathology, biomarker development, and the enhancement of treatment outcomes for patients across various applications. The seamless integration of AI-based solutions throughout the healthcare workflow will be a key driver of AI-enabled advancements in clinical oncology practices. CRISPR-AI is transforming precision medicine by turning CRISPR-Cas systems into powerful, programmable tools for real-time diagnostics, theranostics, and personalized treatments. This integration allows a shift from static testing to adaptive, closed-loop systems that sense molecular signals, interpret disease states, and autonomously guide therapy. AI supports these systems by enhancing gRNA design, predicting off-target effects, deciphering complex biosensor signals, and providing smart decision-making assistance across diverse clinical environments. The adoption of advanced ML techniques, including deep learning, reinforcement learning, generative adversarial networks, and transfer learning, is likely to further improve the accuracy and predictive power of AI models in genomics. Collaboration across disciplines is essential to CRISPR-AI innovation, combining expertise from bioinformatics, molecular biology, computer science, clinical research, and ethics. Establishing dedicated interdisciplinary

research centers can create environments where experts from various fields collaborate on CRISPR-AI projects. In addition, hosting regular conferences and workshops that focus on bridging the gap between disciplines can foster collaboration and knowledge exchange. Encouraging joint academic programs and cross-disciplinary training initiatives will also help build a common language and understanding among researchers from different backgrounds.

Acknowledgement

None.

Financial support

The authors would like to acknowledge funding support from Manipal University Jaipur for the Enhanced Seed Grant under the Endowment Fund (No. E3/2023-24/QE-04-05), as well as the Department of Science & Technology - Fund for Improvement of S&T Infrastructure project (DST/2022/1012) from the Government of India, awarded to the Department of Biosciences, Manipal University Jaipur.

Conflicts of interest statement

The authors declare that they have no competing interests.

Author contributions

Conceptualization: RN; Visualization: BB, CS, PV, RN; Writing—original draft: PV, B, CS, ASK, SKS; Writing—review & editing: AK, RN. All authors have read and agreed to the published version of the manuscript.

Ethics approval and consent to participate

Not applicable.

Consent for publication

Not applicable.

Availability of data

Not applicable.

Open access statement

This is an open-access journal, and articles are distributed under the terms of the Creative Commons Attribution-Non-Commercial-Share Alike 4.0 License, which allows others to remix, tweak, and build upon the work noncommercially if appropriate credit is given. The new creations are licensed under identical terms.

References

- Horvath P, Barrangou R. CRISPR/Cas, the immune system of bacteria and archaea. *Science*. 2010;327(5962):167-170. doi: 10.1126/science.1179555
- Marraffini LA, Sontheimer EJ. CRISPR interference: RNA-directed adaptive immunity in bacteria and archaea. *Nat Rev Genet*. 2010;11(3):181-190. doi: 10.1038/nrg2749
- Allen D, Rosenberg M, Hendel A. Using synthetically engineered guide RNAs to enhance CRISPR genome editing systems in mammalian cells. *Front Genome Ed*. 2021;2:617910. doi: 10.3389/fgeed.2020.617910
- Otoo JA, Schlappi TS. REASSURED multiplex diagnostics: A critical review and forecast. *Biosensors (Basel)*. 2022;12(2):124. doi: 10.3390/bios12020124
- Ochiai H, Yamamoto T. Genome editing using zinc-finger nucleases (ZFNs) and transcription activator-like effector nucleases (TALENs). In: Yamamoto T, editor. *Targeted Genome Editing Using Site-Specific Nucleases: ZFNs, TALENs, and the CRISPR/Cas9 System*. Berlin: Springer Japan; 2015. p. 3-24. doi: 10.1007/978-4-431-55227-7_1
- Reddy P, Vilella F, Izpisua Belmonte JC, Simón C. Use of customizable nucleases for gene editing and other novel applications. *Genes (Basel)*. 2020;11(9):976. doi: 10.3390/genes11090976
- He Y, Yan W, Long L, et al. The CRISPR/Cas system: A customizable toolbox for molecular detection. *Genes (Basel)*. 2023;14(4):850. doi: 10.3390/genes14040850
- O'Connell MR, Oakes BL, Sternberg SH, East-Seletsky A, Kaplan M,

- Doudna JA. Programmable RNA recognition and cleavage by CRISPR/Cas9. *Nature*. 2014;516(7530):263-266. doi: 10.1038/nature13769
9. Mali F. Key socio-economic and (Bio)ethical challenges in the CRISPR-Cas9 patent landscape. In: *Genome Editing in Drug Discovery*. United States: John Wiley & Sons, Ltd.; 2022. p. 315-327. doi: 10.1002/9781119671404.ch21
 10. Yan F, Wang W, Zhang J. CRISPR-Cas12 and Cas13: The lesser known siblings of CRISPR-Cas9. *Cell Biol Toxicol*. 2019;35(6):489-492. doi: 10.1007/s10565-019-09489-1
 11. Zhang L, Jiang H, Zhu Z, Liu J, Li B. Integrating CRISPR/Cas within isothermal amplification for point-of-Care Assay of nucleic acid. *Talanta*. 2022;243:123388. doi: 10.1016/j.talanta.2022.123388
 12. Bhardwaj P, Kant R, Behera SP, Dwivedi GR, Singh R. Next-generation diagnostic with CRISPR/Cas: Beyond nucleic acid detection. *Int J Mol Sci*. 2022;23(11):6052. doi: 10.3390/ijms23116052
 13. Yao J, Yang M, Duan Y. Chemistry, biology, and medicine of fluorescent nanomaterials and related systems: New insights into biosensing, bioimaging, genomics, diagnostics, and therapy. *Chem Rev*. 2014;114(12):6130-6178. doi: 10.1021/cr200359p
 14. Xu Z, Chen D, Li T, et al. Microfluidic space coding for multiplexed nucleic acid detection via CRISPR-Cas12a and recombinase polymerase amplification. *Nat Commun*. 2022;13(1):6480. doi: 10.1038/s41467-022-34086-y
 15. WareJoncas Z, Campbell JM, Martínez-Gálvez G, et al. Precision gene editing technology and applications in nephrology. *Nat Rev Nephrol*. 2018;14(11):663-677. doi: 10.1038/s41581-018-0047-x
 16. Ghavami S, Pandi A. Chapter Five - CRISPR interference and its applications. In: Singh V, editor. *Progress in Molecular Biology and Translational Science. Reprogramming the Genome: Applications of CRISPR-Cas in Non-mammalian Systems Part B*. Vol. 180. United States: Academic Press; 2021. p. 123-140. doi: 10.1016/bs.pmbts.2021.01.007
 17. Safari F, Farajnia S, Ghasemi Y, Zarghami N. New developments in CRISPR technology: Improvements in specificity and efficiency. *Curr Pharm Biotechnol*. 2017;18(13):1038-1054. doi: 10.2174/1389201019666180209120533
 18. Komor AC, Badran AH, Liu DR. Editing the genome without double-stranded DNA breaks. *ACS Chem Biol*. 2018;13(2):383-388. doi: 10.1021/acscmbio.7b00710
 19. Slomovic S, Pardee K, Collins JJ. Synthetic biology devices for *in vitro* and *in vivo* diagnostics. *Proc Natl Acad Sci*. 2015;112(47):14429-14435. doi: 10.1073/pnas.1508521112
 20. Bulle M, Rahman MM, Islam MR, Abbagani S. Strategies to develop climate-resilient chili peppers: Transcription factor optimization through genome editing. *Planta*. 2025;262(2):30. doi: 10.1007/s00425-025-04747-5
 21. Srivastav AK, Mishra MK, Lillard JW, Singh R. Transforming pharmacogenomics and CRISPR gene editing with the power of artificial intelligence for precision medicine. *Pharmaceutics*. 2025;17(5):555. doi: 10.3390/pharmaceutics17050555
 22. Dixit S, Kumar A, Srinivasan K, Vincent PMDR, Ramu Krishnan N. Advancing genome editing with artificial intelligence: Opportunities, challenges, and future directions. *Front Bioeng Biotechnol*. 2024;11:1335901. doi: 10.3389/fbioe.2023.1335901
 23. Srivastava R. Advancing precision oncology with AI-powered genomic analysis. *Front Pharmacol*. 2025;16:1591696. doi: 10.3389/fphar.2025.1591696
 24. Flynn CD, Chang D. Artificial intelligence in point-of-care biosensing: Challenges and opportunities. *Diagnostics (Basel)*. 2024;14(11):1100. doi: 10.3390/diagnostics14111100
 25. Taha BA, Ahmed NM, Talreja RK, et al. Synergizing nanomaterials and artificial intelligence in advanced optical biosensors for precision antimicrobial resistance Diagnosis. *ACS Synth Biol*. 2024;13(6):1600-1620. doi: 10.1021/acssynbio.4c00070
 26. Dara M, Dianatpour M, Azarpira N, Omidifar N. Convergence of CRISPR and artificial intelligence: A paradigm shift in biotechnology. *Human Gene*. 2024;41:201297. doi: 10.1016/j.humgen.2024.201297
 27. Kim H. Overcoming immune barriers in allogeneic CAR-NK therapy: From multiplex gene editing to AI-driven precision design. *Biomolecules*. 2025;15(7):935. doi: 10.3390/biom15070935
 28. Munawar N, Ahmad A. CRISPR/Cas system: An introduction. In: Ahmad A, Khan SH, Khan Z, editors. *CRISPR Crops: The Future of Food Security*. Berlin: Springer; 2021. p. 1-35. doi: 10.1007/978-981-15-7142-8_1
 29. Broeders M, Herrero-Hernandez P, Ernst MPT, Ploeg AT van der, Pijnappel WWMP. Sharpening the molecular scissors: Advances in gene-editing technology. *iScience*. 2020;23(1):100789. doi: 10.1016/j.isci.2019.100789
 30. Liu Y, Pinto F, Wan X, et al. Reprogrammed tracrRNAs enable repurposing of RNAs as crRNAs and sequence-specific RNA biosensors. *Nat Commun*. 2022;13(1):1937. doi: 10.1038/s41467-022-29604-x
 31. Kim HS, Kweon J, Kim Y. Recent advances in CRISPR-based functional genomics for the study of disease-associated genetic variants. *Exp Mol Med*. 2024;56(4):861-869. doi: 10.1038/s12276-024-01212-3
 32. Kolanu ND. CRISPR-Cas9 gene editing: Curing genetic diseases by inherited epigenetic modifications. *Glob Med Genet*. 2024;11(1):113-122. doi: 10.1055/s-0044-1785234
 33. Iranpour S, Abrishami A, Saljooghi AS. Covalent organic frameworks in cancer theranostics: Advancing biomarker detection and tumor-targeted therapy. *Arch Pharm Res*. 2025;48(3):183-211. doi: 10.1007/s12272-025-01536-2
 34. Nidhi S, Anand U, Oleksak P, et al. Novel CRISPR-cas systems: An updated review of the current achievements, applications, and future research perspectives. *Int J Mol Sci*. 2021;22(7):3327. doi: 10.3390/ijms22073327
 35. Schmidt H, Zhang M, Chakarov D, et al. Genome-wide CRISPR guide RNA design and specificity analysis with GuideScan2. *Genome Biol*. 2025;26(1):41. doi: 10.1186/s13059-025-03488-8
 36. Karvelis T, Gasiunas G, Young J, et al. Rapid characterization of CRISPR-Cas9 protospacer adjacent motif sequence elements. *Genome Biol*. 2015;16(1):253. doi: 10.1186/s13059-015-0818-7
 37. Fal K, Carles CC. dCas-based tools to visualize chromatin or modify epigenetic marks at specific plant genomic loci. In: Baroux C, Tatout C, editors. *Methods for Plant Nucleus and Chromatin Studies: Methods and Protocols*. Berlin: Springer US; 2025. p. 305-332. doi: 10.1007/978-1-0716-4228-3_17
 38. Xie J, Huang X, Wang X, et al. ACBE, a new base editor for simultaneous C-to-T and A-to-G substitutions in mammalian systems. *BMC Biol*. 2020;18(1):131. doi: 10.1186/s12915-020-00866-5
 39. Petrova IO, Smirnikhina SA. The development, optimization and future of prime editing. *Int J Mol Sci*. 2023;24(23):17045. doi: 10.3390/ijms242317045
 40. Qi C, Shen X, Li B, et al. PAMPHLET: PAM prediction homologous-enhancement toolkit for precise PAM prediction in CRISPR-Cas systems. *J Genet Genomics*. 2025;52(2):258-268. doi: 10.1016/j.jgg.2024.10.014
 41. Aljabali AAA, El-Tanani M, Tambuwala MM. Principles of CRISPR-Cas9 technology: Advancements in genome editing and emerging trends in drug delivery. *J Drug Deliv Sci Technol*. 2024;92:105338. doi: 10.1016/j.jddst.2024.105338
 42. Habimana JD, Huang R, Muhoza B, et al. Mechanistic insights of CRISPR/Cas nucleases for programmable targeting and early-stage diagnosis: A review. *Biosens Bioelectron*. 2022;203:114033. doi: 10.1016/j.bios.2022.114033
 43. Shihong Gao D, Zhu X, Lu B. Development and application of sensitive, specific, and rapid CRISPR-Cas13-based diagnosis. *J Med Virol*. 2021;93(7):4198-4204. doi: 10.1002/jmv.26889

44. Zhu C, Zhang F, Li H, *et al.* CRISPR/Cas systems accelerating the development of aptasensors. *Trends Anal Chem.* 2023;158:116775. doi: 10.1016/j.trac.2022.116775
45. Hassan YM, Mohamed AS, Hassan YM, El-Sayed WM. Recent developments and future directions in point-of-care next-generation CRISPR-based rapid diagnosis. *Clin Exp Med.* 2025;25(1):33. doi: 10.1007/s10238-024-01540-8
46. Tao J, Bauer DE, Chiarle R. Assessing and advancing the safety of CRISPR-Cas tools: From DNA to RNA editing. *Nat Commun.* 2023;14(1):212. doi: 10.1038/s41467-023-35886-6
47. Bhatia S, Pooja, Yadav SK. CRISPR-Cas for genome editing: Classification, mechanism, designing and applications. *Int J Biol Macromol.* 2023;238:124054. doi: 10.1016/j.ijbiomac.2023.124054
48. Ganger S, Harale G, Majumdar P. Clustered regularly interspaced short palindromic repeats/CRISPR-associated (CRISPR/Cas) systems: Discovery, structure, classification, and general mechanism. In: *CRISPR/Cas-Mediated Genome Editing in Plants*. Burlington: Apple Academic Press; 2023.
49. Liao C, Beisel CL. The tracrRNA in CRISPR biology and technologies. *Annu Rev Genet.* 2021;55:161-181. doi: 10.1146/annurev-genet-071719-022559
50. Wang L, Han H. Strategies for improving the genome-editing efficiency of class 2 CRISPR/Cas system. *Heliyon.* 2024;10(19):e38588. doi: 10.1016/j.heliyon.2024.e38588
51. Tan J, Forner J, Karcher D, Bock R. DNA base editing in nuclear and organellar genomes. *Trends Genet.* 2022;38(11):1147-1169. doi: 10.1016/j.tig.2022.06.015
52. Mistry A, Tanga S, Maji B. Nucleic acid editing. In: Chatterjee S, Chattopadhyay S, editors. *Nucleic Acid Biology and Its Application in Human Diseases*. Berlin: Springer Nature; 2023. p. 365-416. doi: 10.1007/978-981-19-8520-1_11
53. Zhang JH, Adikaram P, Pandey M, Genis A, Simonds WF. Optimization of genome editing through CRISPR-Cas9 engineering. *Bioengineered.* 2016;7(3):166-174. doi: 10.1080/21655979.2016.1189039
54. Ahmad A, Ashraf S, Majeed HN, *et al.* Bioinformatic tools in CRISPR/Cas platform. In: Ahmad A, Khan SH, Khan Z, editors. *The CRISPR/Cas Tool Kit for Genome Editing*. Berlin: Springer; 2022. p. 53-111. doi: 10.1007/978-981-16-6305-5_3
55. Philippidis A. Cloud cover: Benchling expands into early development. *GEN Edge.* 2021;3(1):568-573. doi: 10.1089/genedge.3.1.093
56. Labun K, Montague TG, Krause M, Torres Cleuren YN, Tjeldnes H, Valen E. CHOPCHOP v3: Expanding the CRISPR web toolbox beyond genome editing. *Nucleic Acids Res.* 2019;47(W1):W171-W174. doi: 10.1093/nar/gkz365
57. Kim HK, Min S, Song M, *et al.* Deep learning improves prediction of CRISPR-Cpf1 guide RNA activity. *Nat Biotechnol.* 2018;36(3):239-241. doi: 10.1038/nbt.4061
58. Haeussler M, Schönig K, Eckert H, *et al.* Evaluation of off-target and on-target scoring algorithms and integration into the guide RNA selection tool CRISPOR. *Genome Biol.* 2016;17(1):148. doi: 10.1186/s13059-016-1012-2
59. Heigwer F, Kerr G, Boutros M. E-CRISP: Fast CRISPR target site identification. *Nat Methods.* 2014;11(2):122-123. doi: 10.1038/nmeth.2812
60. McKenna A, Shendure J. FlashFry: A fast and flexible tool for large-scale CRISPR target design. *BMC Biol.* 2018;16(1):74. doi: 10.1186/s12915-018-0545-0
61. Meier JA, Zhang F, Sanjana NE. GUIDES: sgRNA design for loss-of-function screens. *Nat Methods.* 2017;14(9):831-832. doi: 10.1038/nmeth.4423
62. Perez AR, Pritykin Y, Vidigal JA, *et al.* GuideScan software for improved single and paired CRISPR guide RNA design. *Nat Biotechnol.* 2017;35(4):347-349. doi: 10.1038/nbt.3804
63. Hwang GH, Jeong YK, Habib O, *et al.* PE-Designer and PE-Analyzer: Web-based design and analysis tools for CRISPR prime editing. *Nucleic Acids Res.* 2021;49(W1):W499-W504. doi: 10.1093/nar/gkab319
64. Stadager J, Bernardini C, Hartmann L, *et al.* CRISPR GENome and epigenome engineering improves loss-of-function genetic-screening approaches. *Cell Rep Methods.* 2025;5:1-25. doi: 10.1016/j.crmeth.2025.101078
65. Asadbeigi A, Norouzi M, Vafaei Sadi MS, Saffari M, Bakhtiarzadeh MR. CaSilico: A versatile CRISPR package for *in silico* CRISPR RNA designing for Cas12, Cas13, and Cas14. *Front Bioeng Biotechnol.* 2022;10:957131. doi: 10.3389/fbioe.2022.957131
66. Arbab M, Shen MW, Mok B, *et al.* Determinants of base editing outcomes from target library analysis and machine learning. *Cell.* 2020;182(2):463-480.e30. doi: 10.1016/j.cell.2020.05.037
67. Chuai G, Ma H, Yan J, *et al.* DeepCRISPR: Optimized CRISPR guide RNA design by deep learning. *Genome Biol.* 2018;19(1):80. doi: 10.1186/s13059-018-1459-4
68. Schaefer M, Clevert DA, Weiss B, Steffen A. PAVOOC: Designing CRISPR sgRNAs using 3D protein structures and functional domain annotations. *Bioinformatics.* 2019;35(13):2309-2310. doi: 10.1093/bioinformatics/bty935
69. Cancellieri S, Canver MC, Bombieri N, Giugno R, Pinello L. CRISPRitz: Rapid, high-throughput and variant-aware *in silico* off-target site identification for CRISPR genome editing. *Bioinformatics.* 2020;36(7):2001-2008. doi: 10.1093/bioinformatics/btz867
70. Hwang GH, Kim JS, Bae S. Web-based CRISPR toolkits: Cas-OFFinder, cas-designer, and cas-analyzer. In: Fulga TA, Knapp DJHF, Ferry QRV, editors. *CRISPR Guide RNA Design: Methods and Protocols*. Berlin: Springer US; 2021. p. 23-33. doi: 10.1007/978-1-0716-0687-2_2
71. Dobson L, Reményi I, Tusnády GE. CCTOP: A consensus constrained TOPology prediction web server. *Nucleic Acids Res.* 2015;43(W1):W408-W412. doi: 10.1093/nar/gkv451
72. Ma J, Köster J, Qin Q, *et al.* CRISPR-DO for genome-wide CRISPR design and optimization. *Bioinformatics.* 2016;32(21):3336-3338. doi: 10.1093/bioinformatics/btw476
73. sgRNA Scorer 2.0: A Species-Independent Model to Predict CRISPR/Cas9 Activity. *ACS Synthetic Biology*. Available from: <https://pubs.acs.org/doi/abs/10.1021/acssynbio.6b00343> [Last accessed on 2025 Jun 08].
74. Labuhn M, Adams FF, Ng M, *et al.* Refined sgRNA efficacy prediction improves large- and small-scale CRISPR-Cas9 applications. *Nucleic Acids Res.* 2018;46(3):1375-1385. doi: 10.1093/nar/gkx1268
75. Hough SH, Ajetunmbi A, Brody L, Humphries-Kirilov N, Perello E. Desktop genetics. *Person Med.* 2016;13(6):517-521. doi: 10.2217/pme-2016-0068
76. Kearse M, Moir R, Wilson A, *et al.* Geneious Basic: An integrated and extendable desktop software platform for the organization and analysis of sequence data. *Bioinformatics.* 2012;28:1647-1649. doi: 10.1093/bioinformatics/bts199
77. Cross BCS. A power-up for unbiased screening with CRISPR. *Genet Eng Biotechnol News.* 2018;38(18):20-21. doi: 10.1089/gen.38.18.08
78. Pliatsika V, Rigoutsos I. "Off-Spotter": Very fast and exhaustive enumeration of genomic lookalikes for designing CRISPR/Cas guide RNAs. *Biol Direct.* 2015;10(1):4. doi: 10.1186/s13062-015-0035-z
79. Roginsky J. Analyzing CRISPR editing results. *Genet Eng Biotechnol News.* 2018;38(11):S24-S26. doi: 10.1089/gen.38.11.13
80. *Efficient Cas9-based Genome Editing Using CRISPR Analysis Webtools in Severe Early-Onset-Obesity Patient-Derived iPSCs - Patel - 2022 - Current Protocols*. Wiley Online Library. Available from: <https://currentprotocols.onlinelibrary.wiley.com/doi/full/10.1002/cpz1.519> [Last accessed on 2025 Jun 08].
81. Vink JNA, Baijens JHL, Brouns SJJ. PAM-repeat associations and spacer selection preferences in single and co-occurring CRISPR-Cas systems. *Genome Biol.* 2021;22(1):281.

- doi: 10.1186/s13059-021-02495-9
82. Molla KA, Yang Y. CRISPR/Cas-mediated base editing: Technical considerations and practical applications. *Trends Biotechnol.* 2019;37(10):1121-1142. doi: 10.1016/j.tibtech.2019.03.008
 83. Xu Z, Kuang Y, Ren B, et al. SpRY greatly expands the genome editing scope in rice with highly flexible PAM recognition. *Genome Biol.* 2021;22(1):6. doi: 10.1186/s13059-020-02231-9
 84. Wu SS, Li QC, Yin CQ, Xue W, Song CQ. Advances in CRISPR/Cas-based gene therapy in human genetic diseases. *Theranostics.* 2020;10(10):4374-4382. doi: 10.7150/thno.43360
 85. Verma MK, Roychowdhury S, Sahu BD, Mishra A, Sethi KK. CRISPR-based point-of-care diagnostics incorporating Cas9, Cas12, and Cas13 enzymes advanced for SARS-CoV-2 detection. *J Biochem Mol Toxicol.* 2022;36(8):e23113. doi: 10.1002/jbt.23113
 86. Collias D, Beisel CL. CRISPR technologies and the search for the PAM-free nuclease. *Nat Commun.* 2021;12(1):555. doi: 10.1038/s41467-020-20633-y
 87. Mohanraju P, Saha C, van Baarlen P, Louwen R, Staals RHJ, van der Oost J. Alternative functions of CRISPR-Cas systems in the evolutionary arms race. *Nat Rev Microbiol.* 2022;20(6):351-364. doi: 10.1038/s41579-021-00663-z
 88. Zhang XH, Tee LY, Wang XG, Huang QS, Yang SH. Off-target effects in CRISPR/Cas9-mediated genome engineering. *Mol Ther Nucleic Acids.* 2015;4:e264. doi: 10.1038/mtna.2015.37
 89. Singh M, Bindal G, Misra CS, Rath D. The era of Cas12 and Cas13 CRISPR-based disease diagnosis. *Crit Rev Microbiol.* 2022;48(6):714-729. doi: 10.1080/1040841X.2021.2025041
 90. Garrett SC. Pruning and tending immune memories: Spacer dynamics in the CRISPR Array. *Front Microbiol.* 2021;12:664299. doi: 10.3389/fmicb.2021.664299
 91. Hu LF, Li YX, Wang JZ, Zhao YT, Wang Y. Controlling CRISPR-Cas9 by guide RNA engineering. *Wiley Interdiscip Rev RNA.* 2023;14(1):e1731. doi: 10.1002/wrna.1731
 92. Malinin NL, Lee G, Lazzarotto CR, et al. Defining genome-wide CRISPR-Cas genome-editing nuclease activity with GUIDE-seq. *Nat Protoc.* 2021;16(12):5592-5615. doi: 10.1038/s41596-021-00626-x
 93. Ma S, Lv J, Feng Z, Rong Z, Lin Y. Get ready for the CRISPR/Cas system: A beginner's guide to the engineering and design of guide RNAs. *J Gene Med.* 2021;23(11):e3377. doi: 10.1002/jgm.3377
 94. Khan Z, Ali Z, Khan AA, et al. History and classification of CRISPR/Cas system. In: Ahmad A, Khan SH, Khan Z, editors. *The CRISPR/Cas Tool Kit for Genome Editing.* Berlin: Springer; 2022. p. 29-52. doi: 10.1007/978-981-16-6305-5_2
 95. Kasi Viswanath K, Hamid A, Ateka E, Pappu HR. CRISPR/Cas, multiomics, and RNA interference in virus disease management. *Phytopathology.* 2023;113(9):1661-1676. doi: 10.1094/PHYTO-01-23-0002-V
 96. Zhang F, Huang Z. Mechanistic insights into the versatile class II CRISPR toolbox. *Trends Biochem Sci.* 2022;47(5):433-450. doi: 10.1016/j.tibs.2021.11.007
 97. Liu G, Lin Q, Jin S, Gao C. The CRISPR-Cas toolbox and gene editing technologies. *Mol Cell.* 2022;82(2):333-347. doi: 10.1016/j.molcel.2021.12.002
 98. Hillary VE, Ceasar SA. A review on the mechanism and applications of CRISPR/Cas9/Cas12/Cas13/Cas14 proteins utilized for genome engineering. *Mol Biotechnol.* 2023;65(3):311-325. doi: 10.1007/s12033-022-00567-0
 99. Konermann S, Lotfy P, Brideau NJ, Oki J, Shokhirev MN, Hsu PD. Transcriptome engineering with RNA-targeting type VI-D CRISPR effectors. *Cell.* 2018;173(3):665-676.e14. doi: 10.1016/j.cell.2018.02.033
 100. Wu Z, Zhang Y, Yu H, et al. Programmed genome editing by a miniature CRISPR-Cas12f nuclease. *Nat Chem Biol.* 2021;17(11):1132-1138. doi: 10.1038/s41589-021-00868-6
 101. Bonini A, Poma N, Vivaldi F, et al. Advances in biosensing: The CRISPR/Cas system as a new powerful tool for the detection of nucleic acids. *J Pharm Biomed Anal.* 2021;192:113645. doi: 10.1016/j.jpba.2020.113645
 102. Manghwar H, Lindsey K, Zhang X, Jin S. CRISPR/Cas system: Recent advances and future prospects for genome editing. *Trends Plant Sci.* 2019;24(12):1102-1125. doi: 10.1016/j.tplants.2019.09.006
 103. Zhang F. Development of CRISPR-Cas systems for genome editing and beyond. *Q Rev Biophys.* 2019;52:e6. doi: 10.1017/S0033583519000052
 104. Lee H, Sashital DG. Creating memories: Molecular mechanisms of CRISPR adaptation. *Trends Biochem Sci.* 2022;47(6):464-476. doi: 10.1016/j.tibs.2022.02.004
 105. Hille F, Charpentier E. CRISPR-Cas: Biology, mechanisms and relevance. *Philos Trans R Soc Lond B Biol Sci.* 2016;371(1707):20150496. doi: 10.1098/rstb.2015.0496
 106. Asmamaw M, Zawdie B. Mechanism and applications of CRISPR/Cas9-mediated genome editing. *Biologics.* 2021;15:353-361. doi: 10.2147/BTT.S326422
 107. Budhathoki JB, Xiao Y, Schuler G, et al. Real-time observation of CRISPR spacer acquisition by Cas1-Cas2 integrase. *Nat Struct Mol Biol.* 2020;27(5):489-499. doi: 10.1038/s41594-020-0415-7
 108. Qian Y, Zhou D, Li M, et al. Application of CRISPR-Cas system in the diagnosis and therapy of ESKAPE infections. *Front Cell Infect Microbiol.* 2023;13:1223696. doi: 10.3389/fcimb.2023.1223696
 109. Moon SB, Kim DY, Ko JH, Kim JS, Kim YS. Improving CRISPR Genome Editing by Engineering Guide RNAs. *Trends Biotechnol.* 2019;37(8):870-881. doi: 10.1016/j.tibtech.2019.01.009
 110. McCarty NS, Graham AE, Studená L, Ledesma-Amaro R. Multiplexed CRISPR technologies for gene editing and transcriptional regulation. *Nat Commun.* 2020;11(1):1281. doi: 10.1038/s41467-020-15053-x
 111. Rath D, Amlinger L, Rath A, Lundgren M. The CRISPR-Cas immune system: Biology, mechanisms and applications. *Biochimie.* 2015;117:119-128. doi: 10.1016/j.biochi.2015.03.025
 112. Richter C, Chang JT, Fineran PC. Function and regulation of clustered regularly interspaced short palindromic repeats (CRISPR)/CRISPR associated (Cas) systems. *Viruses.* 2012;4(10):2291-2311. doi: 10.3390/v4102291
 113. Javaid N, Choi S. CRISPR/Cas system and factors affecting its precision and efficiency. *Front Cell Dev Biol.* 2021;9:761709. doi: 10.3389/fcell.2021.761709
 114. Deltcheva E, Chylinski K, Sharma CM, et al. CRISPR RNA maturation by trans-encoded small RNA and host factor RNase III. *Nature.* 2011;471(7340):602-607. doi: 10.1038/nature09886
 115. Lau CH, Tin C, Suh Y. CRISPR-based strategies for targeted transgene knock-in and gene correction. *Fac Rev.* 2020;9:20. doi: 10.12703/r/9-20
 116. Chang M, Ahn SJ, Han T, Yang D. Gene expression modulation tools for bacterial synthetic biology. *Biotechnol Sustain Mater.* 2024;1(1):6. doi: 10.1186/s44316-024-00005-y
 117. Semenova E, Jore MM, Datsenko KA, et al. Interference by clustered regularly interspaced short palindromic repeat (CRISPR) RNA is governed by a seed sequence. *Proc Natl Acad Sci.* 2011;108(25):10098-10103. doi: 10.1073/pnas.1104144108
 118. Shalaby K, Aouida M, El-Agnaf O. Tissue-specific delivery of CRISPR therapeutics: Strategies and mechanisms of non-viral vectors. *Int J Mol Sci.* 2020;21(19):7353. doi: 10.3390/ijms21197353
 119. Gupta R, Gupta D, Ahmed KT, et al. Chapter Three - Modification of Cas9, gRNA and PAM: Key to further regulate genome editing and its applications. In: Ghosh D, editor. *Progress in Molecular Biology and Translational Science. Advances in CRISPR/Cas and Related Technologies.*

- Vol. 178. United States: Academic Press; 2021. p. 85-98.
doi: 10.1016/bs.pmbts.2020.12.001
120. Navarro C, Díaz MP, Duran P, *et al.* CRISPR-Cas systems: A functional perspective and innovations. *Int J Mol Sci.* 2025;26(8):3645.
doi: 10.3390/ijms26083645
 121. Lee J, Jeong C. Single-molecule perspectives of CRISPR/Cas systems: Target search, recognition, and cleavage. *BMB Rep.* 2025;58(1):8-16.
doi: 10.5483/BMBRep.2024-0182
 122. Chen J, Chen Y, Huang L, *et al.* Trans-nuclease activity of Cas9 activated by DNA or RNA target binding. *Nat Biotechnol.* 2025;43(4):558-568.
doi: 10.1038/s41587-024-02255-7
 123. Singh J, Liu KG, Allen A, Jiang W, Qin PZ. A DNA unwinding equilibrium serves as a checkpoint for CRISPR-Cas12a target discrimination. *Nucleic Acids Res.* 2023;51(16):8730-8743.
doi: 10.1093/nar/gkad636
 124. Pacesa M, Loeff L, Querques I, Muckenfuss LM, Sawicka M, Jinek M. R-loop formation and conformational activation mechanisms of Cas9. *Nature.* 2022;609(7925):191-196.
doi: 10.1038/s41586-022-05114-0
 125. Kordyś M, Sen R, Warkocki Z. Applications of the versatile CRISPR-Cas13 RNA targeting system. *Wiley Interdiscip Rev RNA.* 2022;13(3):e1694.
doi: 10.1002/wrna.1694
 126. Wang JY, Pausch P, Doudna JA. Structural biology of CRISPR-Cas immunity and genome editing enzymes. *Nat Rev Microbiol.* 2022;20(11):641-656.
doi: 10.1038/s41579-022-00739-4
 127. Gunitseva N, Evteeva M, Borisova A, Patrushev M, Subach F. RNA-dependent RNA targeting by CRISPR-Cas systems: Characterizations and applications. *Int J Mol Sci.* 2023;24(8):6894.
doi: 10.3390/ijms24086894
 128. Jeon Y, Choi YH, Jang Y, *et al.* Direct observation of DNA target searching and cleavage by CRISPR-Cas12a. *Nat Commun.* 2018;9(1):2777.
doi: 10.1038/s41467-018-05245-x
 129. Li H, Yang Y, Hong W, Huang M, Wu M, Zhao X. Applications of genome editing technology in the targeted therapy of human diseases: Mechanisms, advances and prospects. *Sig Transduct Target Ther.* 2020;5(1):1.
doi: 10.1038/s41392-019-0089-y
 130. Singh S, Chaudhary R, Deshmukh R, Tiwari S. Opportunities and challenges with CRISPR-Cas mediated homologous recombination based precise editing in plants and animals. *Plant Mol Biol.* 2023;111(1):1-20.
doi: 10.1007/s11103-022-01321-5
 131. Park SH, Cao M, Bao G. Detection and quantification of unintended large on-target gene modifications due to CRISPR/Cas9 editing. *Curr Opin Biomed Eng.* 2023;28:100478.
doi: 10.1016/j.cobme.2023.100478
 132. Ahmad A, Rasheed M, Ashraf S, *et al.* Beyond traditional gene editing: Expanding applications of CRISPR-Cas. In: *Gene-Edited Crops*. United States: CRC Press; 2025.
 133. Xu X, Qi LS. A CRISPR-dCas toolbox for genetic engineering and synthetic biology. *J Mol Biol.* 2019;431(1):34-47.
doi: 10.1016/j.jmb.2018.06.037
 134. Kazi TA, Biswas SR. Chapter Four - CRISPR/dCas system as the modulator of gene expression. In: Ghosh D, editor. *Progress in Molecular Biology and Translational Science. Advances in CRISPR/Cas and Related Technologies*. Vol. 178. United States: Academic Press; 2021. p. 99-122.
doi: 10.1016/bs.pmbts.2020.12.002
 135. Nissim L, Perli SD, Fridkin A, Perez-Pinera P, Lu TK. Multiplexed and programmable regulation of gene networks with an integrated RNA and CRISPR/Cas toolkit in human cells. *Mol Cell.* 2014;54(4):698-710.
doi: 10.1016/j.molcel.2014.04.022
 136. Pandya K, Jagani D, Singh N. CRISPR-Cas systems: Programmable nuclease revolutionizing the molecular diagnosis. *Mol Biotechnol.* 2024;66(8):1739-1753.
doi: 10.1007/s12033-023-00819-7
 137. Sohail M, Xie S, Zhang X, Li B. Methodologies in visualizing the activation of CRISPR/Cas: The last mile in developing CRISPR-Based diagnostics and biosensing - A review. *Anal Chim Acta.* 2022;1205:339541.
doi: 10.1016/j.aca.2022.339541
 138. Pardee K, Green AA, Takahashi MK, *et al.* Rapid, low-cost detection of zika virus using programmable biomolecular components. *Cell.* 2016;165(5):1255-1266.
doi: 10.1016/j.cell.2016.04.059
 139. Zhou W, Hu L, Ying L, Zhao Z, Chu PK, Yu XF. A CRISPR-Cas9-triggered strand displacement amplification method for ultrasensitive DNA detection. *Nat Commun.* 2018;9(1):5012.
doi: 10.1038/s41467-018-07324-5
 140. Huang M, Zhou X, Wang H, Xing D. Clustered regularly interspaced short palindromic repeats/Cas9 triggered isothermal amplification for site-specific nucleic acid detection. *Anal Chem.* 2018;90(3):2193-2200.
doi: 10.1021/acs.analchem.7b04542
 141. Wang X, Xiong E, Tian T, *et al.* Clustered regularly interspaced short palindromic repeats/Cas9-mediated lateral flow nucleic acid assay. *ACS Nano.* 2020;14(2):2497-2508.
doi: 10.1021/acsnano.0c00022
 142. Azhar M, Phutela R, Kumar M, *et al.* Rapid and accurate nucleobase detection using FnCas9 and its application in COVID-19 diagnosis. *Biosens Bioelectron.* 2021;183:113207.
doi: 10.1016/j.bios.2021.113207
 143. Hajian R, Balderston S, Tran T, *et al.* Detection of unamplified target genes via CRISPR-Cas9 immobilized on a graphene field-effect transistor. *Nat Biomed Eng.* 2019;3(6):427-437.
doi: 10.1038/s41551-019-0371-x
 144. Quan J, Langelier C, Kuchta A, *et al.* FLASH: A next-generation CRISPR diagnostic for multiplexed detection of antimicrobial resistance sequences. *Nucleic Acids Res.* 2019;47(14):e83.
doi: 10.1093/nar/gkz418
 145. Wang T, Liu Y, Sun HH, Yin BC, Ye BC. An RNA-guided Cas9 nickase-based method for universal isothermal DNA amplification. *Angew Chem.* 2019;131(16):5436-5440.
doi: 10.1002/ange.201901292
 146. Tsou JH, Leng Q, Jiang F. A CRISPR test for detection of circulating nuclei acids. *Transl Oncol.* 2019;12(12):1566-1573.
doi: 10.1016/j.tranon.2019.08.011
 147. Li SY, Cheng QX, Wang JM, *et al.* CRISPR-Cas12a-assisted nucleic acid detection. *Cell Discov.* 2018;4:20.
doi: 10.1038/s41421-018-0028-z
 148. Dai Y, Somoza RA, Wang L, *et al.* Exploring the trans-cleavage activity of CRISPR-Cas12a (cpf1) for the development of a universal electrochemical biosensor. *Angew Chem Int Ed Engl.* 2019;58(48):17399-17405.
doi: 10.1002/anie.201910772
 149. Compiro P, Chomta N, Nimnual J, *et al.* CRISPR-Cas12a-based detection and differentiation of *Mycobacterium* spp. *Clin Chim Acta.* 2025;567:120101.
doi: 10.1016/j.cca.2024.120101
 150. Teng F, Guo L, Cui T, *et al.* CDetection: CRISPR-Cas12b-based DNA detection with sub-attomolar sensitivity and single-base specificity. *Genome Biol.* 2019;20(1):132.
doi: 10.1186/s13059-019-1742-z
 151. Li L, Li S, Wu N, *et al.* HOLMESv2: A CRISPR-Cas12b-assisted platform for nucleic acid detection and DNA methylation quantitation. *ACS Synth Biol.* 2019;8(10):2228-2237.
doi: 10.1021/acssynbio.9b00209
 152. Harrington LB, Burstein D, Chen JS, *et al.* Programmed DNA destruction by miniature CRISPR-Cas14 enzymes. *Science.* 2018;362(6416):839-842.
doi: 10.1126/science.aav4294
 153. Huang Z, Fang J, Zhou M, Gong Z, Xiang T. CRISPR-Cas13: A new technology for the rapid detection of pathogenic microorganisms. *Front Microbiol.* 2022;13:1011399.
doi: 10.3389/fmicb.2022.1011399
 154. Gootenberg JS, Abudayyeh OO, Kellner MJ, Joung J, Collins JJ, Zhang F. Multiplexed and portable nucleic acid detection platform with Cas13, Cas12a, and Csm6. *Science.* 2018;360(6387):439-444.
doi: 10.1126/science.aaq0179
 155. Aralis Z, Rauch JN, Audouard M, *et al.* CREST, a Cas13-based, rugged, equitable, scalable testing (CREST) for SARS-CoV-2 detection in patient samples. *Curr Protoc.* 2022;2(2):e385.
doi: 10.1002/cpz1.385
 156. Katzmeier F, Aufinger L, Dupin A, *et al.* A low-cost fluorescence reader for in vitro transcription and nucleic acid detection with Cas13a. *PLoS*

- One*. 2019;14(12):e0220091.
doi: 10.1371/journal.pone.0220091
157. Freije CA, Myhrvold C, Boehm CK, et al. Programmable inhibition and detection of RNA viruses using Cas13. *Mol Cell*. 2019;76(5):826-837.e11.
doi: 10.1016/j.molcel.2019.09.013
 158. Arizti-Sanz J, Freije CA, Stanton AC, et al. Streamlined inactivation, amplification, and Cas13-based detection of SARS-CoV-2. *Nat Commun*. 2020;11(1):5921.
doi: 10.1038/s41467-020-19097-x
 159. Zhou T, Huang R, Huang M, Shen J, Shan Y, Xing D. CRISPR/Cas13a powered portable electrochemiluminescence chip for ultrasensitive and specific MiRNA detection. *Adv Sci*. 2020;7(13):1903661.
doi: 10.1002/adv.201903661
 160. Wang Y, Li H, Luo S, Zhong M, Liu J, Li B. Research progress on signal conversion based on aptamer combined CRISPR/Cas system in biosensors. *Mol Diagn Ther*. 2025;29(4):499-518.
doi: 10.1007/s40291-025-00785-7
 161. Feng Y, Liu S, Chen R, Xie A. Target binding and residence: A new determinant of DNA double-strand break repair pathway choice in CRISPR/Cas9 genome editing. *J Zhejiang Univ Sci B*. 2021;22(1):73-86.
doi: 10.1631/jzus.B2000282
 162. Qian S, Chen Y, Xu X, et al. Advances in amplification-free detection of nucleic acid: CRISPR/Cas system as a powerful tool. *Anal Biochem*. 2022;643:114593.
doi: 10.1016/j.ab.2022.114593
 163. Zhu R, Jiang H, Li C, et al. CRISPR/Cas9-based point-of-care lateral flow biosensor with improved performance for rapid and robust detection of *Mycoplasma pneumoniae*. *Anal Chim Acta*. 2023;1257:341175.
doi: 10.1016/j.aca.2023.341175
 164. Ali Z, Sánchez E, Tehseen M, et al. Bio-SCAN: A CRISPR/dCas9-based lateral flow assay for rapid, specific, and sensitive detection of SARS-CoV-2. *ACS Synth Biol*. 2022;11(1):406-419.
doi: 10.1021/acssynbio.1c00499
 165. Zhai S, Yang Y, Wu Y, et al. A visual CRISPR/dCas9-mediated enzyme-linked immunosorbent assay for nucleic acid detection with single-base specificity. *Talanta*. 2023;257:124318.
doi: 10.1016/j.talanta.2023.124318
 166. Agha ASAA, Al-Samydai A, Aburjai T. New frontiers in CRISPR: Addressing antimicrobial resistance with Cas9, Cas12, Cas13, and Cas14. *Heliyon*. 2025;11(2):e42013.
doi: 10.1016/j.heliyon.2025.e42013
 167. Hadi J, Rapp D, Dhawan S, Gupta SK, Gupta TB, Brightwell G. Molecular detection and characterization of foodborne bacteria: Recent progresses and remaining challenges. *Compr Rev Food Sci Food Saf*. 2023;22(3):2433-2464.
doi: 10.1111/1541-4337.13153
 168. Hadi R, Poddar A, Sonnila S, Bhavaraju VSM, Agrawal S. Advancing CRISPR-based solutions for COVID-19 diagnosis and therapeutics. *Cells*. 2024;13(21):1794.
doi: 10.3390/cells13211794
 169. Chatterjee P, Jakimo N, Jacobson JM. Minimal PAM specificity of a highly similar SpCas9 ortholog. *Sci Adv*. 2018;4(10):eaau0766.
doi: 10.1126/sciadv.aau0766
 170. Hirano H, Gootenberg JS, Horii T, et al. Structure and engineering of *Francisella novicida* Cas9. *Cell*. 2016;164(5):950-961.
doi: 10.1016/j.cell.2016.01.039
 171. Azhar Mohd, Phutela R, Kumar M, et al. Rapid and accurate nucleobase detection using FnCas9 and its application in COVID-19 diagnosis. *Biosens Bioelectron*. 2021;183:113207.
doi: 10.1016/j.bios.2021.113207
 172. Kumar M, Gulati S, Ansari AH, et al. FnCas9-based CRISPR diagnostic for rapid and accurate detection of major SARS-CoV-2 variants on a paper strip. *Elife*. 2021;10:e67130.
doi: 10.7554/eLife.67130
 173. Kaminski MM, Abudayyeh OO, Gootenberg JS, Zhang F, Collins JJ. CRISPR-based diagnostics. *Nat Biomed Eng*. 2021;5(7):643-656.
doi: 10.1038/s41551-021-00760-7
 174. Chakraborty S. Democratizing nucleic acid-based molecular diagnostic tests for infectious diseases at resource-limited settings - from point of care to extreme point of care. *Sens Diagn*. 2024;3(4):536-561.
doi: 10.1039/D3SD00304C
 175. Wang T, Wang Z, Bai L, et al. Next-generation CRISPR-based diagnostic tools for human diseases. *Trends Anal Chem*. 2023;168:117328.
doi: 10.1016/j.trac.2023.117328
 176. Swarts DC, Jinek M. Mechanistic insights into the cis- and trans-acting DNase activities of Cas12a. *Mol Cell*. 2019;73(3):589-600.e4.
doi: 10.1016/j.molcel.2018.11.021
 177. Swarts DC. Making the cut(s): How Cas12a cleaves target and non-target DNA. *Biochem Soc Trans*. 2019;47(5):1499-1510.
doi: 10.1042/BST20190564
 178. Wang SY, Du YC, Wang DX, Ma JY, Tang AN, Kong DM. Signal amplification and output of CRISPR/Cas-based biosensing systems: A review. *Anal Chim Acta*. 2021;1185:338882.
doi: 10.1016/j.aca.2021.338882
 179. Broughton JP, Deng X, Yu G, et al. CRISPR-Cas12-based detection of SARS-CoV-2. *Nat Biotechnol*. 2020;38(7):870-874.
doi: 10.1038/s41587-020-0513-4
 180. Yu L, Peng Y, Sheng M, Wang Q, Huang J, Yang X. Sensitive and amplification-free electrochemiluminescence biosensor for HPV-16 detection based on CRISPR/Cas12a and DNA tetrahedron nanostructures. *ACS Sens*. 2023;8(7):2852-2858.
doi: 10.1021/acssensors.3c00806
 181. Luo T, Li J, He Y, et al. Designing a CRISPR/Cas12a- and Au-nanobeacon-based diagnostic biosensor enabling direct, rapid, and sensitive miRNA detection. *Anal Chem*. 2022;94(17):6566-6573.
doi: 10.1021/acs.analchem.2c00401
 182. Gao H, Zhang H, Qi X, et al. CRISPR/Cas12a dual-mode biosensor for *Staphylococcus aureus* detection via enzyme-free isothermal amplification. *Talanta*. 2025;282:127013.
doi: 10.1016/j.talanta.2024.127013
 183. Taufiq S, Nagata M, Abbas SR, Sode K. An electrochemical biosensor for the detection of tuberculosis specific DNA with CRISPR-Cas12a and redox-probe modified oligonucleotide. *Heliyon*. 2024;10(23):e40754.
doi: 10.1016/j.heliyon.2024.e40754
 184. Liu P, Wang X, Liang J, et al. A recombinase polymerase amplification-coupled Cas12a mutant-based module for efficient detection of streptomycin-resistant mutations in *Mycobacterium tuberculosis*. *Front Microbiol*. 2022;12:796916.
doi: 10.3389/fmicb.2021.796916
 185. Yee BJ, Shafiqah NF, Mohd-Naim NF, Ahmed MU. A CRISPR/Cas12a-based fluorescence aptasensor for the rapid and sensitive detection of ampicillin. *Int J Biol Macromol*. 2023;242:125211.
doi: 10.1016/j.ijbiomac.2023.125211
 186. Xu J, Zhang T, Lv X, Shi L, Bai W, Ye L. An RPA-based CRISPR/Cas12a assay in combination with a lateral flow assay for the rapid detection of *Shigella flexneri* in food samples. *Foods*. 2024;13(19):3200.
doi: 10.3390/foods13193200
 187. *Sherlock Biosciences. The Future of Molecular Diagnostics*. Sherlock Biosciences. Available from: <https://sherlock.bio> [Last accessed on 2025 Jul 16].
 188. *Mammoth Biosciences. Mammoth Biosciences*. Available from: <https://mammoth.bio> [Last accessed on 2025 Jul 16].
 189. *Innovating for Human Well-Being*. Available from: <https://crisprbits.com> [Last accessed on 2025 Jul 16].
 190. *CASPR Biotech. SOSV*. Available from: <https://sosv.com/company/caspr-biotech> [Last accessed on 2025 Jul 16].
 191. *Scope Biosciences*. Available from: <https://scopebio.com> [Last accessed on 2025 Jul 16].
 192. *Home - Locus Biosciences. Locus Bioscience*. Available from: <https://www.locus-bio.com> [Last accessed on 2025 Jul 16].
 193. *MEDiC*. Available from: <https://www.medic-life-sciences.com> [Last accessed on 2025 Jul 16].
 194. *CRISPR Products For Gene Editing*. IDT. Available from: <https://www.idtdna.com/page/products/crispr-genome-editing> [Last accessed on 2025 Jul 16].
 195. *Build Your own CRISPR Solution - in*. Available from: <https://www.thermofisher.com/in/en/home/life-science/genome-editing/crispr-nuclease-vector.html> [Last accessed on 2025 Jul 16].
 196. *Takara Bio-Home*. Available from: <https://www.takarabio.com> [Last accessed on 2025 Jul 16].

197. Information about CRISPR-Cpf1 (Cas12a) Systems; 2017. Available from: <https://www.broadinstitute.org/crispr/information-about-crispr-cpf1-cas12a-systems> [Last accessed on 2025 Jul 16].
198. Repare Therapeutics. *Synthetic Lethality Precision Oncology. Repare Therapeutics*. Available from: <https://www.reparerx.com> [Last accessed on 2025 Jul 16].
199. Home - KSQ Therapeutics. Available from: <https://ksqtx.com> [Last accessed on 2025 Jul 16].
200. Preclinical Oncology CRO. Contract Research Drug Development Company. Available from: <https://www.crownbio.com> [Last accessed on 2025 Jul 16].
201. Freenome Outpacing Cancer Starts with Early Detection. Freenome. Available from: <https://www.freenome.com> [Last accessed on 2025 Jul 16].
202. Guardant Health. *Conquering Cancer With Data*. Guardant Health. Available from: <https://guardanthealth.com> [Last accessed on 2025 Jul 16].
203. Natera: A Global Leader in cfDNA Testing. Natera. Available from: <https://www.natera.com> [Last accessed on 2025 Jul 16].
204. Cardea Bio. Serra Ventures, LLC. Available from: <https://www.serraventures.com/cardea-bio-1> [Last accessed on 2025 Jul 16].
205. Home. Ginkgo Bioworks. Available from: <https://ginkgo.bio> [Last accessed on 2025 Jul 16].
206. Caribou Biosciences. *Developing Sophisticated Allogeneic Cell Therapies*. Available from: <https://www.cariboubio.com> [Last accessed on 2025 Jul 16].
207. Ghounemy A, Mahas A, Marsic T, Aman R, Mahfouz M. CRISPR-based diagnostics: Challenges and potential solutions toward point-of-care applications. *ACS Synth Biol*. 2023;12(1):1-16. doi: 10.1021/acssynbio.2c00496
208. O'Connell MR. Molecular mechanisms of RNA targeting by Cas13-containing Type VI CRISPR-Cas systems. *J Mol Biol*. 2019;431(1):66-87. doi: 10.1016/j.jmb.2018.06.029
209. Granados-Riveron JT, Aquino-Jarquín G. CRISPR/Cas13-based approaches for ultrasensitive and specific detection of microRNAs. *Cells*. 2021;10(7):1655. doi: 10.3390/cells10071655
210. Zhao L, Qiu M, Li X, Yang J, Li J. CRISPR-Cas13a system: A novel tool for molecular diagnostics. *Front Microbiol*. 2022;13:1060947. doi: 10.3389/fmicb.2022.1060947
211. Ramadan NK, Gaber N, Ali NM, Amer OSO, Soliman H. SHERLOCK, a novel CRISPR-Cas13a-based assay for detection of infectious bursal disease virus. *J Virol Methods*. 2025;337:115185. doi: 10.1016/j.jviromet.2025.115185
212. Cunningham CH, Hennelly CM, Lin JT, et al. A novel CRISPR-based malaria diagnostic capable of *Plasmodium* detection, species differentiation, and drug-resistance genotyping. *EBioMedicine*. 2021;68:103415. doi: 10.1016/j.ebiom.2021.103415
213. Ackerman CM, Myhrvold C, Thakku SG, et al. Massively multiplexed nucleic acid detection with Cas13. *Nature*. 2020;582(7811):277-282. doi: 10.1038/s41586-020-2279-8
214. Yin X, Luo H, Zhou H, et al. A rapid isothermal CRISPR-Cas13a diagnostic test for genital herpes simplex virus infection. *iScience*. 2024;27(1):108581. doi: 10.1016/j.isci.2023.108581
215. Sheng Y, Zhang T, Zhang S, et al. A CRISPR/Cas13a-powered catalytic electrochemical biosensor for successive and highly sensitive RNA diagnostics. *Biosens Bioelectron*. 2021;178:113027. doi: 10.1016/j.bios.2021.113027
216. Jiang L, Du J, Xu H, et al. Ultrasensitive CRISPR/Cas13a-mediated photoelectrochemical biosensors for specific and direct assay of miRNA-21. *Anal Chem*. 2023;95(2):1193-1200. doi: 10.1021/acs.analchem.2c03945
217. Kumar M, Maiti S, Chakraborty D. Capturing nucleic acid variants with precision using CRISPR diagnostics. *Biosens Bioelectron*. 2022;217:114712. doi: 10.1016/j.bios.2022.114712
218. Mao X, Xu M, Luo S, et al. Advancements in the synergy of isothermal amplification and CRISPR-cas technologies for pathogen detection. *Front Bioeng Biotechnol*. 2023;11:1273988. doi: 10.3389/fbioe.2023.1273988
219. Azeez SS, Hamad RS, Hamad BK, Shekha MS, Bergsten P. Advances in CRISPR-Cas technology and its applications: Revolutionising precision medicine. *Front Genome Ed*. 2024;6:1509924. doi: 10.3389/fgeed.2024.1509924
220. Ci Q, He Y, Chen J. Novel Anti-CRISPR-assisted CRISPR biosensor for exclusive detection of single-stranded DNA (ssDNA). *ACS Sens*. 2024;9(3):1162-1167. doi: 10.1021/acssensors.4c00201
221. Shi R, Zhong L, Liu G, Mak WC. CRISPR/Cas biosensing technology: From lab assays to integrated portable devices towards wearables. *Trends Anal Chem*. 2024;177:117796. doi: 10.1016/j.trac.2024.117796
222. Wang Y, Peng Y, Zhou H, Gao Z. A universal CRISPR-Cas14a responsive triple-sensitized upconversion photoelectrochemical sensor. *J Nanobiotechnol*. 2023;21(1):389. doi: 10.1186/s12951-023-02163-z
223. Qi J, Qi Q, Zhou Z, et al. PER-CRISPR/Cas14a system-based electrochemical biosensor for the detection of ctDNA EGFR L858R. *Anal Methods*. 2024;16(1):51-61. doi: 10.1039/D3AY01615C
224. Li C, Liu C, Liu R, et al. A novel CRISPR/Cas14a-based electrochemical biosensor for ultrasensitive detection of *Burkholderia pseudomallei* with PtPd@PCN-224 nanoenzymes for signal amplification. *Biosens Bioelectron*. 2023;225:115098. doi: 10.1016/j.bios.2023.115098
225. Huang S, Dai R, Zhang Z, et al. CRISPR/Cas-based techniques for live-cell imaging and bioanalysis. *Int J Mol Sci*. 2023;24(17):13447. doi: 10.3390/ijms241713447
226. Zhou B, Yang R, Sohail M, et al. CRISPR/Cas14 provides a promising platform in facile and versatile aptasensing with improved sensitivity. *Talanta*. 2023;254:124120. doi: 10.1016/j.talanta.2022.124120
227. Philippidis A. Mammoth pursues coronavirus partnership as it grows CRISPR ambitions. *GEN Edge*. 2020. doi: 10.1089/genedge.2.1.11
228. van Dongen JE, Berendsen JTW, Steenbergen RDM, Wolthuis RMF, Eijkel JCT, Segerink LI. Point-of-care CRISPR/Cas nucleic acid detection: Recent advances, challenges and opportunities. *Biosens Bioelectron*. 2020;166:112445. doi: 10.1016/j.bios.2020.112445
229. Naresh V, Lee N. A review on biosensors and recent development of nanostructured materials-enabled biosensors. *Sensors (Basel)*. 2021;21(4):1109. doi: 10.3390/s21041109
230. Li H, Xie Y, Chen F, et al. Amplification-free CRISPR/Cas detection technology: Challenges, strategies, and perspectives. *Chem Soc Rev*. 2023;52(1):361-382. doi: 10.1039/D2CS00594H
231. Zhang Z, Hu JJ, Lin S, Wu J, Xia F, Lou X. Field effect transistor biosensors for healthcare monitoring. *Interdiscip Med*. 2024;2(4):e20240032. doi: 10.1002/INMD.20240032
232. Zhou J, Li Z, Olajide JS, Wang G. CRISPR/Cas-based nucleic acid detection strategies: Trends and challenges. *Heliyon*. 2024;10(4):e26179. doi: 10.1016/j.heliyon.2024.e26179
233. Cheng X, Li Y, Kou J, et al. Novel non-nucleic acid targets detection strategies based on CRISPR/Cas toolboxes: A review. *Biosens Bioelectron*. 2022;215:114559. doi: 10.1016/j.bios.2022.114559
234. Li Y, Zhao L, Ma L, Bai Y, Feng F. CRISPR/Cas and argonate-powered lateral flow assay for pathogens detection. *Crit Rev Food Sci Nutr*. 2025;65:5464-5468. doi: 10.1080/10408398.2024.2416473
235. Conference proceedings - 4th international conference on molecular diagnostics and biomarker discovery: Antibody technology. *BMC Proc*. 2019;13(8):10. doi: 10.1186/s12919-019-0169-6
236. Lino C, Barrias S, Chaves R, Adegá F, Martins-Lopes P, Fernandes JR. Biosensors as diagnostic tools in clinical applications. *Biochim Biophys Acta Rev Cancer*. 2022;1877(3):188726. doi: 10.1016/j.bbcan.2022.188726

237. Razavi Z, Soltani M, Souri M, Pazoki-Toroudi H. CRISPR-driven biosensors: A new frontier in rapid and accurate disease detection. *Crit Rev Anal Chem.* 2024;Sep 17:1-25. doi: 10.1080/10408347.2024.2400267
238. Kumaran A, Jude Serpes N, Gupta T, et al. Advancements in CRISPR-based biosensing for next-gen point of care diagnostic application. *Biosensors (Basel).* 2023;13(2):202. doi: 10.3390/bios13020202
239. Zavvar TS, Khoshbin Z, Ramezani M, Alibolandi M, Abnous K, Taghdisi SM. CRISPR/Cas-engineered technology: Innovative approach for biosensor development. *Biosens Bioelectron.* 2022;214:114501. doi: 10.1016/j.bios.2022.114501
240. Dronina J, Samukaite-Bubniene U, Ramanavicius A. Towards application of CRISPR-Cas12a in the design of modern viral DNA detection tools (Review). *J Nanobiotechnol.* 2022;20(1):41. doi: 10.1186/s12951-022-01246-7
241. Gattani A, Mandal S, Agrawal A, et al. CRISPR-based electrochemical biosensors for animal health: Recent advances. *Prog Biophys Mol Biol.* 2024;193:7-18. doi: 10.1016/j.pbiomolbio.2024.09.001
242. Wachholz Junior D, Kubota LT. CRISPR-based electrochemical biosensors: An alternative for point-of-care diagnostics? *Talanta.* 2024;278:126467. doi: 10.1016/j.talanta.2024.126467
243. Duan H, Wang Y, Tang SY, Xiao TH, Goda K, Li M. A CRISPR-Cas12a powered electrochemical sensor based on gold nanoparticles and MXene composite for enhanced nucleic acid detection. *Sens Actuat B Chem.* 2023;380:133342. doi: 10.1016/j.snb.2023.133342
244. Wan Y, Zong C, Li X, et al. New insights for biosensing: Lessons from microbial defense systems. *Chem Rev.* 2022;122(9):8126-8180. doi: 10.1021/acs.chemrev.1c01063
245. Kadam US, Cho Y, Park TY, Hong JC. Aptamer-based CRISPR-Cas powered diagnostics of diverse biomarkers and small molecule targets. *Appl Biol Chem.* 2023;66(1):13. doi: 10.1186/s13765-023-00771-9
246. Chen A, Shah B. Electrochemical sensing and biosensing based on square wave voltammetry. *Anal Methods.* 2013;5(9):2158-2173. doi: 10.1039/C3AY40155C
247. Randviir EP, Banks CE. A review of electrochemical impedance spectroscopy for bioanalytical sensors. *Anal Methods.* 2022;14(45):4602-4624. doi: 10.1039/D2AY00970F
248. He C, Li Y, Liu J, et al. Application of CRISPR-Cas system in human papillomavirus detection using biosensor devices and point-of-care technologies. *BME Front.* 2025;6:0114. doi: 10.34133/bmef.0114
249. Li L, Gopinath SCB, Lakshmi Priya T, Subramaniam S, Anbu P. Zeolite-iron oxide integrated integrated electrode sensor for diagnosing cervical cancer. *Heliyon.* 2024;10(11):e31851. doi: 10.1016/j.heliyon.2024.e31851
250. Ma J, Li X, Lou C, et al. Utility of CRISPR/Cas mediated electrochemical biosensors. *Anal Methods.* 2023;15(31):3785-3801. doi: 10.1039/D3AY00903C
251. Dhar BC, Steimberg N, Mazzoleni G. Point-of-care pathogen detection with CRISPR-based programmable nucleic acid binding proteins. *ChemMedChem.* 2021;16(10):1566-1575. doi: 10.1002/cmdc.202000782
252. Del Giovane S, Bagheri N, Di Pedic AC, et al. Challenges and perspectives of CRISPR-based technology for diagnostic applications. *Trends Anal Chem.* 2024;172:117594. doi: 10.1016/j.trac.2024.117594
253. Yang Y, Li X, Wang X, Wang Z, Gong S. CRISPR-Cas-based colorimetric strategies for nucleic acids detection. *Trends Anal Chem.* 2025;182:118058. doi: 10.1016/j.trac.2024.118058
254. Son H. Harnessing CRISPR/Cas systems for DNA and RNA detection: Principles, techniques, and challenges. *Biosensors (Basel).* 2024;14(10):460. doi: 10.3390/bios14100460
255. Xiao M, Tian F, Liu X, et al. Virus detection: From state-of-the-art laboratories to smartphone-based point-of-care testing. *Adv Sci.* 2022;9(17):2105904. doi: 10.1002/advs.202105904
256. Abdolhosseini M, Zandsalimi F, Moghaddam FS, Tavoosidana G. A review on colorimetric assays for DNA virus detection. *J Virol Methods.* 2022;301:114461. doi: 10.1016/j.jviromet.2022.114461
257. Alizadeh N, Salimi A, Hallaj R. Hemin/G-quadruplex horseradish peroxidase-mimicking DNAzyme: Principle and biosensing application. In: Seitz H, Stahl F, Walter JG, editors. *Catalytically Active Nucleic Acids.* Berlin: Springer International Publishing; 2020. p. 85-106. doi: 10.1007/10_2017_37
258. Ferrari E. Gold nanoparticle-based plasmonic biosensors. *Biosensors (Basel).* 2023;13(3):411. doi: 10.3390/bios13030411
259. Zhang WS, Pan J, Li F, et al. Reverse transcription recombinase polymerase amplification coupled with CRISPR-Cas12a for facile and highly sensitive colorimetric SARS-CoV-2 detection. *Anal Chem.* 2021;93(8):4126-4133. doi: 10.1021/acs.analchem.1c00013
260. Wang Y, Peng Y, Li S, et al. The development of a fluorescence/colorimetric biosensor based on the cleavage activity of CRISPR-Cas12a for the detection of non-nucleic acid targets. *J Hazard Mater.* 2023;449:131044. doi: 10.1016/j.jhazmat.2023.131044
261. Aiamsa-at P, Nonthakaew N, Phiwisaiya K, Senapin S, Chaijarasphong T. CRISPR-based, genotype-specific detection of yellow head virus genotype 1 with fluorescent, lateral flow and DNAzyme-assisted colorimetric readouts. *Aquaculture.* 2023;574:739696. doi: 10.1016/j.aquaculture.2023.739696
262. Jin X, Zhu J, Zhang Y, et al. The CRISPR/Cas system-mediated function of Hg²⁺ on urease activity for colorimetric detection of the tumor biomarker in clinical samples. *Microchemical J.* 2025;208:112317. doi: 10.1016/j.microc.2024.112317
263. Saleh EAM, Ali E, Muxamadovna GM, et al. CRISPR/Cas-based colorimetric biosensors: A promising tool for the diagnosis of bacterial foodborne pathogens in food products. *Anal Methods.* 2024;16(22):3448-3463. doi: 10.1039/D4AY00578C
264. Li X, Liu M, Men D, et al. Rapid, portable, and sensitive detection of CaMV35S by RPA-CRISPR/Cas12a-G4 colorimetric assays with high accuracy deep learning object recognition and classification. *Talanta.* 2024;278:126441. doi: 10.1016/j.talanta.2024.126441
265. Liu J, Wachsmann-Hogiu S. Progress and challenges of point-of-need photonic biosensors for the diagnosis of COVID-19 infections and immunity. *Biosensors (Basel).* 2022;12(9):678. doi: 10.3390/bios12090678
266. Kelly T, Yang X. Application of fluorescence- and bioluminescence-based biosensors in cancer drug discovery. *Biosensors (Basel).* 2024;14(12):570. doi: 10.3390/bios14120570
267. Xie S, Ji Z, Suo T, Li B, Zhang X. Advancing sensing technology with CRISPR: From the detection of nucleic acids to a broad range of analytes – A review. *Anal Chim Acta.* 2021;1185:338848. doi: 10.1016/j.aca.2021.338848
268. Huang Z, Liu S, Pei X, et al. Fluorescence signal-readout of CRISPR/Cas biosensors for nucleic acid detection. *Biosensors (Basel).* 2022;12(10):779. doi: 10.3390/bios12100779
269. Feng W, Zhang H, Le XC. Signal amplification by the trans-cleavage activity of CRISPR-Cas systems: Kinetics and performance. *Anal Chem.* 2023;95(1):206-217. doi: 10.1021/acs.analchem.2c04555
270. Fang C, Huang Y, Zhao Y. Review of FRET biosensing and its application in biomolecular detection. *Am J Transl Res.* 2023;15(2):694-709.
271. Fang X, Zheng Y, Duan Y, Liu Y, Zhong W. Recent advances in design of fluorescence-based assays for high-throughput screening. *Anal Chem.* 2019;91(1):482-504. doi: 10.1021/acs.analchem.8b05303
272. Mohammadi R, Naderi-Manesh H, Farzin L, et al. Fluorescence sensing and imaging with carbon-based quantum dots for early diagnosis of

- cancer: A review. *J Pharm Biomed Anal.* 2022;212:114628. doi: 10.1016/j.jpba.2022.114628
273. Song C, Ye Z, Wang G, Yuan J, Guan Y. Core-shell nanoarchitectures: A strategy to improve the efficiency of luminescence resonance energy transfer. *ACS Nano.* 2010;4(9):5389-5397. doi: 10.1021/nn100820u
274. Cao X, Chen C, Zhu Q. Biosensors based on functional nucleic acids and isothermal amplification techniques. *Talanta.* 2023;253:123977. doi: 10.1016/j.talanta.2022.123977
275. Liu BM. Isothermal nucleic acid amplification technologies and CRISPR-Cas-based nucleic acid detection strategies for infectious diseases diagnostics. In: *Manual of Molecular Microbiology.* United States: John Wiley & Sons, Ltd.; 2025. p. 30-47. doi: 10.1002/9781683674597.ch3
276. Mukherjee A, Samanta S, Das S, et al. Leveraging CRISPR-Cas-enhanced isothermal amplification tools for quick identification of pathogens causing livestock diseases. *Curr Microbiol.* 2025;82(6):260. doi: 10.1007/s00284-025-04226-w
277. Srivastava P, Prasad D. Isothermal nucleic acid amplification and its uses in modern diagnostic technologies. *3 Biotech.* 2023;13(6):200. doi: 10.1007/s13205-023-03628-6
278. Wang M, Liu H, Ren J, et al. Enzyme-assisted nucleic acid amplification in molecular diagnosis: A review. *Biosensors (Basel).* 2023;13(2):160. doi: 10.3390/bios13020160
279. Kulkarni A, Tanga S, Karmakar A, Hota A, Maji B. CRISPR-based precision molecular diagnostics for disease detection and surveillance. *ACS Appl Bio Mater.* 2023;6(10):3927-3945. doi: 10.1021/acsabm.3c00439
280. Zahra A, Shahid A, Shamim A, Khan SH, Arshad MI. The SHERLOCK platform: An insight into advances in viral disease diagnosis. *Mol Biotechnol.* 2023;65(5):699-714. doi: 10.1007/s12033-022-00625-7
281. Barnes KG, Lachenauer AE, Nitido A, et al. Deployable CRISPR-Cas13a diagnostic tools to detect and report Ebola and Lassa virus cases in real-time. *Nat Commun.* 2020;11(1):4131. doi: 10.1038/s41467-020-17994-9
282. Qiao J, Zhang J, Jiang Q, et al. Boosting CRISPR/Cas12a intrinsic RNA detection capability through pseudo hybrid DNA-RNA substrate design. *Nucleic Acids Res.* 2025;53(11):gkaf510. doi: 10.1093/nar/gkaf510
283. Calabretta MM, Gregucci D, Martínez-Pérez-Cejuela H, Michelini E. A Luciferase mutant with improved brightness and stability for whole-cell bioluminescent biosensors and *in vitro* biosensing. *Biosensors (Basel).* 2022;12(9):742. doi: 10.3390/bios12090742
284. Yeh HW, Ai HW. Development and applications of bioluminescent and chemiluminescent reporters and biosensors. *Annu Rev Anal Chem.* 2019;12:129-150. doi: 10.1146/annurev-anchem-061318-115027
285. Singhal SS, Garg R, Mohanty A, et al. Recent advancement in breast cancer research: Insights from model organisms-mouse models to zebrafish. *Cancers (Basel).* 2023;15(11):2961. doi: 10.3390/cancers15112961
286. Deng P, Dong XC, Wang XY, Gao YP, Quan FS. Verification of CRISPR/Cas9 activity *in vitro* via SSA-based dual-luciferase reporter System. *Mol Biol.* 2024;58(3):461-470. doi: 10.1134/S0026893324700092
287. Krissanaprasit A, Key CM, Pontula S, LaBean TH. Self-assembling nucleic acid nanostructures functionalized with aptamers. *Chem Rev.* 2021;121(22):13797-13868. doi: 10.1021/acs.chemrev.0c01332
288. Chen K, Zhu L, Li J, et al. High-content tailoring strategy to improve the multifunctionality of functional nucleic acids. *Biosens Bioelectron.* 2024;261:116494. doi: 10.1016/j.bios.2024.116494
289. Zhu F, Zhao Q. CRISPR/Cas12a linked sandwich aptamer assay for sensitive detection of thrombin. *Anal Chim Acta.* 2024;1287:342106. doi: 10.1016/j.aca.2023.342106
290. Qing M, Sun Z, Wang L, et al. CRISPR/Cas12a-regulated homogeneous electrochemical aptasensor for amplified detection of protein. *Sens Actuat B Chem.* 2021;348:130713. doi: 10.1016/j.snb.2021.130713
291. Song J, Song Y, Jang H, et al. Elution-free DNA detection using CRISPR/Cas9-mediated light-up aptamer transcription: Toward all-in-one DNA purification and detection tube. *Biosens Bioelectron.* 2023;225:115085. doi: 10.1016/j.bios.2023.115085
292. Sun H, Wang N, Zhang L, Meng H, Li Z. Aptamer-Based Sensors for Thrombin Detection Application. *Chemosensors.* 2022;10(7):255. doi: 10.3390/chemosensors10070255
293. Guan X, Zhao J, Sha Z, et al. CRISPR/Cas12a and aptamer-chemiluminescence based analysis for the relative abundance determination of tumor-related protein positive exosomes for breast cancer diagnosis. *Biosens Bioelectron.* 2024;259:116380. doi: 10.1016/j.bios.2024.116380
294. Liu L, Han Z, An F, et al. Aptamer-based biosensors for the diagnosis of sepsis. *J Nanobiotechnol.* 2021;19(1):216. doi: 10.1186/s12951-021-00959-5
295. Léguillier V, Heddi B, Vidic J. Recent advances in aptamer-based biosensors for bacterial detection. *Biosensors (Basel).* 2024;14(5):210. doi: 10.3390/bios14050210
296. Mondal B, Ramlal S, Lavu PS, Bhavanashri N, Kingston J. Highly sensitive colorimetric biosensor for staphylococcal enterotoxin B by a label-free aptamer and gold nanoparticles. *Front Microbiol.* 2018;9. doi: 10.3389/fmicb.2018.00179
297. Urmi R, Banerjee P, Singh M, et al. Revolutionizing biomedicine: Aptamer-based nanomaterials and nanodevices for therapeutic applications. *Biotechnol Rep.* 2024;42:e00843. doi: 10.1016/j.btre.2024.e00843
298. Lakhin AV, Tarantul VZ, Gening LV. Aptamers: Problems, solutions and prospects. *Acta Naturae.* 2013;5(4):34-43.
299. Chowdhry R, Lu SZ, Lee S, Godhulayyagari S, Ebrahimi SB, Samanta D. Enhancing CRISPR/Cas systems with nanotechnology. *Trends Biotechnol.* 2023;41(12):1549-1564. doi: 10.1016/j.tibtech.2023.06.005
300. Hii ARK, Qi X, Wu Z. Advanced strategies for CRISPR/Cas9 delivery and applications in gene editing, therapy, and cancer detection using nanoparticles and nanocarriers. *J Mater Chem B.* 2024;12(6):1467-1489. doi: 10.1039/D3TB01850D
301. Huang Y, Wen Q, Xiong Y, et al. Nanomaterials driven CRISPR/Cas-based biosensing strategies. *Chem Eng J.* 2023;474:145615. doi: 10.1016/j.cej.2023.145615
302. Peng W, Shi M, Hu B, et al. Nanotechnology-leveraged CRISPR/Cas systems: Icebreaking in trace cancer-related nucleic acids biosensing. *Mol Cancer.* 2025;24(1):78. doi: 10.1186/s12943-024-02222-5
303. Sun T, He W, Chen X, Shu X, Liu W, Ouyang G. Nanomaterials-integrated CRISPR/Cas systems: Expanding the toolbox for optical detection. *ACS Sens.* 2025;10(4):2453-2473. doi: 10.1021/acssensors.5c00020
304. Kim D, Le QV, Wu Y, Park J, Oh YK. Nanovesicle-mediated delivery systems for CRISPR/Cas genome editing. *Pharmaceutics.* 2020;12(12):1233. doi: 10.3390/pharmaceutics12121233
305. Xu X, Liu C, Wang Y, et al. Nanotechnology-based delivery of CRISPR/Cas9 for cancer treatment. *Adv Drug Deliv Rev.* 2021;176:113891. doi: 10.1016/j.addr.2021.113891
306. Wang M, Jin L, Hang-Mei Leung P, et al. Advancements in magnetic nanoparticle-based biosensors for point-of-care testing. *Front Bioeng Biotechnol.* 2024;12:1393789. doi: 10.3389/fbioe.2024.1393789
307. Park DH, Haizan I, Ahn MJ, Choi MY, Kim MJ, Choi JH. One-Pot CRISPR-Cas12a-Based Viral DNA detection via HRP-enriched extended ssDNA-modified Au@Fe₃O₄ nanoparticles. *Biosensors.* 2024;14(1):26. doi: 10.3390/bios14010026
308. Liu L, Xu Z, Awayda K, et al. Gold nanoparticle-labeled CRISPR-Cas13a assay for the sensitive solid-state nanopore molecular counting. *Adv Mater Technol.* 2022;7(3):2101550. doi: 10.1002/admt.202101550
309. Osborn MJ, Bhardwaj A, Bingea SP, et al. CRISPR/Cas9-based lateral flow and fluorescence diagnostics. *Bioengineering (Basel).* 2021;8(2):23.

- doi: 10.3390/bioengineering8020023
310. Yin H, Sun L, Pu Y, et al. Ultrasound-controlled CRISPR/Cas9 system augments sonodynamic therapy of hepatocellular carcinoma. *ACS Cent Sci.* 2021;7(12):2049-2062. doi: 10.1021/acscentsci.1c01143
 311. Nsairat H, Alshaer W, Odeh F, et al. Recent advances in using liposomes for delivery of nucleic acid-based therapeutics. *OpenNano.* 2023;11:100132. doi: 10.1016/j.onano.2023.100132
 312. Zakari S, Niels NK, Olagunju GV, et al. Emerging biomarkers for non-invasive diagnosis and treatment of cancer: A systematic review. *Front Oncol.* 2024;14:1405267. doi: 10.3389/fonc.2024.1405267
 313. Shetti D, Mallela VR, Ye W, et al. Emerging role of circulating cell-free RNA as a non-invasive biomarker for hepatocellular carcinoma. *Crit Rev Oncol Hematol.* 2024;200:104391. doi: 10.1016/j.critrevonc.2024.104391
 314. Toden S, Goel A. Non-coding RNAs as liquid biopsy biomarkers in cancer. *Br J Cancer.* 2022;126(3):351-360. doi: 10.1038/s41416-021-01672-8
 315. Shahni SN, Albogami S, Pattnaik B, et al. CRISPR-Cas12a based detection of EGFR gene mutation in cell free DNA for early diagnosis of non-small cell lung cancer (NSCLC). *Sens Biosens Res.* 2025;47:100735. doi: 10.1016/j.sbsr.2025.100735
 316. Yang J, Lin N, Niu M, Yin B. Circulating tumor DNA mutation analysis: Advances in its application for early diagnosis of hepatocellular carcinoma and therapeutic efficacy monitoring. *Aging (Albany NY).* 2024;16(14):11460-11474. doi: 10.18632/aging.205980
 317. Kumar MA, Baba SK, Sadida HQ, et al. Extracellular vesicles as tools and targets in therapy for diseases. *Sig Transduct Target Ther.* 2024;9(1):27. doi: 10.1038/s41392-024-01735-1
 318. Zhao Z, Zhao G, Yang S, Zhu S, Zhang S, Li P. The significance of exosomal RNAs in the development, diagnosis, and treatment of pancreatic cancer. *Cancer Cell Int.* 2021;21(1):364. doi: 10.1186/s12935-021-02059-8
 319. Porzycki P, Ciszakowicz E, Semik M, Tyrka M. Combination of three miRNA (miR-141, miR-21, and miR-375) as potential diagnostic tool for prostate cancer recognition. *Int Urol Nephrol.* 2018;50(9):1619-1626. doi: 10.1007/s11255-018-1938-2
 320. Song K, Han C, Dash S, Balart LA, Wu T. MiR-122 in hepatitis B virus and hepatitis C virus dual infection. *World J Hepatol.* 2015;7(3):498-506. doi: 10.4254/wjh.v7.i3.498
 321. Pacesa M, Pelea O, Jinek M. Past, present, and future of CRISPR genome editing technologies. *Cell.* 2024;187(5):1076-1100. doi: 10.1016/j.cell.2024.01.042
 322. Lee M, Lee M, Song Y, Kim S, Park N. Recent advances and prospects of nucleic acid therapeutics for anti-cancer therapy. *Molecules.* 2024;29(19):4737. doi: 10.3390/molecules29194737
 323. Song N, Chu Y, Li S, et al. A dual-enzyme-responsive DNA-based nanoframework enables controlled co-delivery of CRISPR-Cas9 and antisense oligodeoxynucleotide for synergistic gene therapy. *Adv Funct Mater.* 2023;33(47):2306634. doi: 10.1002/adfm.202306634
 324. Lyu M, Kong L, Yang Z, Wu Y, McGhee CE, Lu Y. PNA-Assisted DNazymes to cleave double-stranded DNA for genetic engineering with high sequence fidelity. *J Am Chem Soc.* 2021;143(26):9724-9728. doi: 10.1021/jacs.1c03129
 325. Stovicek V, Holkenbrink C, Borodina I. CRISPR/Cas system for yeast genome engineering: Advances and applications. *FEMS Yeast Res.* 2017;17(5):fox030. doi: 10.1093/femsyr/fox030
 326. Stace LB. Point-of-care testing in primary care. In: John RM, editor. *Pediatric Diagnostic Labs for Primary Care: An Evidence-Based Approach.* Berlin: Springer International Publishing; 2022. p. 135-169. doi: 10.1007/978-3-030-90642-9_5
 327. Little P, Hobbs FDR, Moore M, et al. Clinical score and rapid antigen detection test to guide antibiotic use for sore throats: Randomised controlled trial of PRISM (primary care streptococcal management). *BMJ.* 2013;347:f5806. doi: 10.1136/bmj.f5806
 328. Jarnda KV, Dai H, Ali A, et al. A review on optical biosensors for monitoring of uric acid and blood glucose using portable POCT Devices: Status, challenges, and future horizons. *Biosensors (Basel).* 2025;15(4):222. doi: 10.3390/bios15040222
 329. Bao C, Liu X, Liang C, Xu S. CRISPR/Cas-SERS sensing platforms: A frontier technology for next-generation fast, low-cost, ultra-micro biosample detection. *J Raman Spectrosc.* doi: 10.1002/jrs.6827
 330. Broughton JP, Deng X, Yu G, et al. Rapid detection of 2019 novel coronavirus SARS-CoV-2 using a CRISPR-based DETECTR Lateral Flow Assay. *medRxiv.* 2020. doi: 10.1101/2020.03.06.20032334
 331. Joung J, Ladha A, Saito M, et al. Point-of-care testing for COVID-19 using SHERLOCK diagnostics. *medRxiv.* 2020. doi: 10.1101/2020.05.04.20091231
 332. Kellner MJ, Koob JG, Gootenberg JS, Abudayyeh OO, Zhang F. SHERLOCK: Nucleic acid detection with CRISPR nucleases. *Nat Protoc.* 2019;14(10):2986-3012. doi: 10.1038/s41596-019-0210-2
 333. Antropov DN, Stepanov GA. Molecular mechanisms underlying CRISPR/Cas-based assays for nucleic acid detection. *Curr Issues Mol Biol.* 2023;45(1):649-662. doi: 10.3390/cimb45010043
 334. Li Y, Liu Y, Tang X, et al. CRISPR/Cas-powered amplification-free detection of nucleic acids: Current state of the art, challenges, and futuristic perspectives. *ACS Sens.* 2023;8(12):4420-4441. doi: 10.1021/acssensors.3c01463
 335. Tian Z, Yan H, Zeng Y. Solid-phase extraction and enhanced amplification-free detection of pathogens integrated by multifunctional CRISPR-Cas12a. *ACS Appl Mater Interfaces.* 2024;16(12):14445-14456. doi: 10.1021/acsaami.3c17039
 336. Lau CH, Huang S, Zhu H. Amplification-free nucleic acids detection with next-generation CRISPR/dx systems. *Crit Rev Biotechnol.* 2025;45(4):859-886. doi: 10.1080/07388551.2024.2399560
 337. Liu Q, Jin X, Cheng J, Zhou H, Zhang Y, Dai Y. Advances in the application of molecular diagnostic techniques for the detection of infectious disease pathogens (Review). *Mol Med Rep.* 2023;27(5):104. doi: 10.3892/mmr.2023.12991
 338. de Puig H, Lee RA, Najjar D, et al. Minimally instrumented SHERLOCK (miSHERLOCK) for CRISPR-based point-of-care diagnosis of SARS-CoV-2 and emerging variants. *Sci Adv.* 2021;7(32):eabh2944. doi: 10.1126/sciadv.abh2944
 339. Fermann GJ, Suyama J. Point of care testing in the emergency department. *J Emerg Med.* 2002;22(4):393-404. doi: 10.1016/S0736-4679(02)00429-8
 340. Razavi Z, Soltani M, Pazoki-Toroudi H, Chen P. CRISPR-microfluidics nexus: Advancing biomedical applications for understanding and detection. *Sens Actuat A Phys.* 2024;376:115625. doi: 10.1016/j.sna.2024.115625
 341. Chan KG, Ang GY, Yu CY, Yean CY. Harnessing CRISPR-Cas to combat COVID-19: From diagnostics to therapeutics. *Life (Basel).* 2021;11(11):1210. doi: 10.3390/life11111210
 342. Li Z, Ding X, Yin K, Avery L, Ballesteros E, Liu C. Instrument-free, CRISPR-based diagnostics of SARS-CoV-2 using self-contained microfluidic system. *Biosens Bioelectron.* 2022;199:113865. doi: 10.1016/j.bios.2021.113865
 343. Ngamsom B, Iles A, Kamita M, et al. An integrated lab-on-a-chip device for RNA extraction, amplification and CRISPR-Cas12a-assisted detection for COVID-19 screening in resource-limited settings. *medRxiv.* 2022. doi: 10.1101/2022.01.06.22268835
 344. Kalligosfyri PM, Lamprou E, Kalogianni DP. Emerging sensing technologies for liquid biopsy applications: Steps closer to personalized medicine. *Sensors (Basel).* 2024;24(24):7902. doi: 10.3390/s24247902
 345. Neumann F, Madaboosi N, Nilsson M. Isothermal amplification methods for point-of-care diagnostics of infectious diseases. In: *Emerging*

- Technologies in Biophysical Sciences: A World Scientific Reference*. USA: World Scientific; 2020. p. 239-286.
doi: 10.1142/9789811226113_0009
346. Yang B, Kong J, Fang X. Programmable CRISPR-Cas9 microneedle patch for long-term capture and real-time monitoring of universal cell-free DNA. *Nat Commun*. 2022;13(1):3999.
doi: 10.1038/s41467-022-31740-3
 347. Jiang Q, Mo Q, Ge C, et al. Applications of artificial intelligence-driven microfluidics in medical laboratory science. *Interdiscip Med*. 2025;3:e20240135.
doi: 10.1002/INMD.20240135
 348. van Dongen JE, Segerink LI. Building the future of clinical diagnostics: An analysis of potential benefits and current barriers in CRISPR/Cas diagnostics. *ACS Synth Biol*. 2025;14(2):323-331.
doi: 10.1021/acssynbio.4c00816
 349. Umar Ibrahim A, Pwavodi CP, Ozsoz M, Al-Turjman F, Galaya T, Agbo JJ. Crispr biosensing and Ai driven tools for detection and prediction of Covid-19. *J Exp Theor Art Intell*. 2023;35(4):489-505.
doi: 10.1080/0952813X.2021.1952652
 350. Dave S, Dave A, Radhakrishnan S, Das J, Dave S. Chapter 16 - Biosensors for healthcare: An artificial intelligence approach. In: Das J, Dave S, Radhakrishnan S, Mohanty P, editors. *Biosensors for Emerging and Re-Emerging Infectious Diseases*. United States: Academic Press; 2022. p. 365-383.
doi: 10.1016/B978-0-323-88464-8.00008-7
 351. Lee M. Deep learning in CRISPR-Cas systems: A review of recent studies. *Front Bioeng Biotechnol*. 2023;11:1226182.
doi: 10.3389/fbioe.2023.1226182
 352. Baker DV, Bernal-Escalante J, Traaseth C, et al. Smartphones as a platform for molecular analysis: Concepts, methods, devices and future potential. *Lab Chip*. 2025;25(5):884-955.
doi: 10.1039/D4LC00966E
 353. Zhong Z, Li Z, Yang J, Wang Q. Unified model to predict gRNA efficiency across diverse cell lines and CRISPR-Cas9 systems. *J Chem Inf Model*. 2023;63(23):7320-7329.
doi: 10.1021/acs.jcim.3c01339
 354. Konstantakos V, Nentidis A, Krithara A, Paliouras G. CRISPR-Cas9 gRNA efficiency prediction: An overview of predictive tools and the role of deep learning. *Nucleic Acids Res*. 2022;50(7):3616-3637.
doi: 10.1093/nar/gkac192
 355. Manghwar H, Li B, Ding X, et al. CRISPR/Cas systems in genome editing: Methodologies and tools for sgRNA design, off-target evaluation, and strategies to mitigate off-target effects. *Adv Sci (Weinh)*. 2020;7(6):1902312.
doi: 10.1002/advs.201902312
 356. Liu Q, Cheng X, Liu G, Li B, Liu X. Deep learning improves the ability of sgRNA off-target propensity prediction. *BMC Bioinformatics*. 2020;21(1):51.
doi: 10.1186/s12859-020-3395-z
 357. Li T, Cheng N. Sensitive and portable signal readout strategies boost point-of-care CRISPR/Cas12a biosensors. *ACS Sens*. 2023;8(11):3988-4007.
doi: 10.1021/acssensors.3c01338
 358. Liu L, Pei DS. Insights gained from RNA editing targeted by the CRISPR-Cas13 family. *Int J Mol Sci*. 2022;23(19):11400.
doi: 10.3390/ijms231911400
 359. Zhang C, Yang Y, Qi T, et al. Prediction of base editor off-targets by deep learning. *Nat Commun*. 2023;14(1):5358.
doi: 10.1038/s41467-023-41004-3
 360. Schene IF, Joore IP, Oka R, et al. Prime editing for functional repair in patient-derived disease models. *Nat Commun*. 2020;11(1):5352.
doi: 10.1038/s41467-020-19136-7
 361. Han GR, Goncharov A, Eryilmaz M, et al. Machine learning in point-of-care testing: Innovations, challenges, and opportunities. *Nat Commun*. 2025;16(1):3165.
doi: 10.1038/s41467-025-58527-6
 362. Moingeon P, Kuenemann M, Guedj M. Artificial intelligence-enhanced drug design and development: Toward a computational precision medicine. *Drug Discov Today*. 2022;27(1):215-222.
doi: 10.1016/j.drudis.2021.09.006
 363. Yang Q, Dong MJ, Xu J, et al. CRISPR/RNA aptamer system activated by an AND logic gate for biomarker-driven theranostics. *J Am Chem Soc*. 2025;147(1):169-180.
doi: 10.1021/jacs.4c08719
 364. Lai YH, Sun SC, Chuang MC. Biosensors with built-in biomolecular logic gates for practical applications. *Biosensors (Basel)*. 2014;4(3):273-300.
doi: 10.3390/bios4030273
 365. Chen YM, Hsiao TH, Lin CH, Fann YC. Unlocking precision medicine: Clinical applications of integrating health records, genetics, and immunology through artificial intelligence. *J Biomed Sci*. 2025;32(1):16.
doi: 10.1186/s12929-024-01110-w
 366. O'Leary TJ, O'Leary BJ, O'Leary DP. A perspective on artificial intelligence for molecular pathologists. *J Mol Diagn*. 2025;27(5):323-335.
doi: 10.1016/j.jmoldx.2025.01.005
 367. Gao S, Fang A, Huang Y, et al. Empowering biomedical discovery with AI agents. *Cell*. 2024;187(22):6125-6151.
doi: 10.1016/j.cell.2024.09.022
 368. Yadav N, Narang J, Chhillar AK, Rana JS. CRISPR: A new paradigm of theranostics. *Nanomedicine*. 2021;33:102350.
doi: 10.1016/j.nano.2020.102350
 369. Li SY, Cheng QX, Liu JK, Nie XQ, Zhao GP, Wang J. CRISPR-Cas12a has both cis- and trans-cleavage activities on single-stranded DNA. *Cell Res*. 2018;28(4):491-493.
doi: 10.1038/s41422-018-0022-x
 370. Dominguez AA, Lim WA, Qi LS. Beyond editing: repurposing CRISPR-Cas9 for precision genome regulation and interrogation. *Nat Rev Mol Cell Biol*. 2016;17(1):5-15.
doi: 10.1038/nrm.2015.2
 371. Pun FW, Ozerov IV, Zhavoronkov A. AI-powered therapeutic target discovery. *Trends Pharmacol Sci*. 2023;44(9):561-572.
doi: 10.1016/j.tips.2023.06.010
 372. Akhtar M, Nehal N, Gull A, et al. Explicating the transformative role of artificial intelligence in designing targeted nanomedicine. *Expert Opin Drug Deliv*. 2025;22(7):971-991.
doi: 10.1080/17425247.2025.2502022
 373. Sergeeva OV, Luo L, Guiseppi-Elie A. Cancer theragnostics: closing the loop for advanced personalized cancer treatment through the platform integration of therapeutics and diagnostics. *Front Bioeng Biotechnol*. 2025;12:1499474.
doi: 10.3389/fbioe.2024.1499474
 374. Park SH, Bao G. CRISPR/Cas9 gene editing for curing sickle cell disease. *Transfus Apher Sci*. 2021;60(1):103060.
doi: 10.1016/j.transci.2021.103060
 375. Liu F, Peng J, Lei YM, et al. Electrochemical detection of ctDNA mutation in non-small cell lung cancer based on CRISPR/Cas12a system. *Sens Actuat B Chem*. 2022;362:131807.
doi: 10.1016/j.snb.2022.131807
 376. Jiang H, Xi H, Juhas M, Zhang Y. Biosensors for point mutation detection. *Front Bioeng Biotechnol*. 2021;9:797831.
doi: 10.3389/fbioe.2021.797831
 377. Tsou JH, Leng Q, Jiang F. A CRISPR test for rapidly and sensitively detecting circulating EGFR mutations. *Diagnostics (Basel)*. 2020;10(2):114.
doi: 10.3390/diagnostics10020114
 378. Wilbie D, Walther J, Mastrobattista E. Delivery aspects of CRISPR/Cas for *in vivo* genome editing. *Acc Chem Res*. 2019;52(6):1555-1564.
doi: 10.1021/acs.accounts.9b00106
 379. Bendixen L, Jensen TI, Bak RO. CRISPR-Cas-mediated transcriptional modulation: The therapeutic promises of CRISPRa and CRISPRi. *Mol Ther*. 2023;31(7):1920-1937.
doi: 10.1016/j.ymthe.2023.03.024
 380. Lee MH, Thomas JL, Lin CY, Li YCE, Lin HY. Activation of insulin gene expression via transfection of a CRISPR/dCas9a system using magnetic peptide-imprinted nanoparticles. *Pharmaceutics*. 2023;15(4):1311.
doi: 10.3390/pharmaceutics15041311
 381. Kang H, Park D, Kim J. Logical regulation of endogenous gene expression using programmable, multi-input processing CRISPR guide RNAs. *Nucleic Acids Res*. 2024;52(14):8595-8608.
doi: 10.1093/nar/gkae549
 382. Sheth RU, Yim SS, Wu FL, Wang HH. Multiplex recording of cellular events over time into a CRISPR biological tape. *Science*. 2017;358(6369):1457-1461.

- doi: 10.1126/science.aao0958
383. Jia AY, Kiess AP, Li Q, Antonarakis ES. Radiotheranostics in advanced prostate cancer: Current and future directions. *Prostate Cancer Prostatic Dis.* 2024;27(1):11-21.
doi: 10.1038/s41391-023-00670-6
 384. Kostyusheva A, Brezgin S, Babin Y, et al. CRISPR-Cas systems for diagnosing infectious diseases. *Methods.* 2022;203:431-446.
doi: 10.1016/j.ymeth.2021.04.007
 385. Janowicz PW, Boele T, Maschmeyer RT, et al. Enhanced detection of glioblastoma vasculature with superparamagnetic iron oxide nanoparticles and MRI. *Sci Rep.* 2025;15(1):14283.
doi: 10.1038/s41598-025-97943-y
 386. Jackson BR, Sendak MP, Solomonides A, Balu S, Sittig DF. Regulation of artificial intelligence in healthcare: Clinical Laboratory Improvement Amendments (CLIA) as a model. *J Am Med Inform Assoc.* 2025;32(2):404-407.
doi: 10.1093/jamia/ocae296
 387. Niazi SK. The coming of age of AI/ML in drug discovery, development, clinical testing, and manufacturing: The FDA perspectives. *Drug Design Dev Ther.* 2023;17:2691-2725.
doi: 10.2147/DDDT.S424991
 388. World Health Organization. *2023 Emerging Technologies and Scientific Innovations: A Global Public Health Perspective.* Geneva: World Health Organization; 2023.
 389. Li L, Mandal PK. Recent advancements in gene therapy for sickle cell disease and β -thalassemia. *Front Hematol.* 2024;3:1468952.
doi: 10.3389/frhem.2024.1468952
 390. Zeng S, Lei S, Qu C, Wang Y, Teng S, Huang P. CRISPR/Cas-based gene editing in therapeutic strategies for beta-thalassemia. *Hum Genet.* 2023;142(12):1677-1703.
doi: 10.1007/s00439-023-02610-9
 391. Khoshandam M, Soltaninejad H, Hamidieh AA, Hosseinkhani S. CRISPR, CAR-T, and NK: Current applications and future perspectives. *Genes Dis.* 2024;11(4):101121.
doi: 10.1016/j.gendis.2023.101121
 392. Wang Y, Zafar N, Ali Q, et al. CRISPR/Cas genome editing technologies for plant improvement against biotic and abiotic stresses: Advances, limitations, and future perspectives. *Cells.* 2022;11(23):3928.
doi: 10.3390/cells11233928
 393. Agrawal R. Emerging technologies for improvement of microbial strains using omic sciences and measuring methods for maximum product formation. In: Agrawal R, editor. *Textbook of Industrial Microbiology.* Berlin: Springer Nature; 2024. p. 13-39.
doi: 10.1007/978-981-97-9582-6_2
 394. Matinvafa MA, Makani S, Parsasharif N, Zahed MA, Movahed E, Ghiasvand S. CRISPR-Cas technology secures sustainability through its applications: A review in green biotechnology. *3 Biotech.* 2023;13(11):383.
doi: 10.1007/s13205-023-03786-7
 395. Sadanov AK, Baimakhanova BB, Orasymbet SE, et al. Engineering useful microbial species for pharmaceutical applications. *Microorganisms.* 2025;13(3):599.
doi: 10.3390/microorganisms13030599
 396. Cardiff RAL, Carothers JM, Zalatan JG, Sauro HM. Systems-level modeling for CRISPR-based metabolic engineering. *ACS Synth Biol.* 2024;13(9):2643-2652.
doi: 10.1021/acssynbio.4c00053
 397. Li Y, Lin Z, Huang C, et al. Metabolic engineering of *Escherichia coli* using CRISPR-Cas9 mediated genome editing. *Metabolic Eng.* 2015;31:13-21.
doi: 10.1016/j.ymben.2015.06.006
 398. Lu L, Shen X, Sun X, Yan Y, Wang J, Yuan Q. CRISPR-based metabolic engineering in non-model microorganisms. *Curr Opin Biotechnol.* 2022;75:102698.
doi: 10.1016/j.copbio.2022.102698
 399. Zhao D, Zhu X, Zhou H, et al. CRISPR-based metabolic pathway engineering. *Metab Eng.* 2021;63:148-159.
doi: 10.1016/j.ymben.2020.10.004
 400. Herrera ML, Paraiso-Luna J, Bustos-Martínez I, Barco Á. Targeting epigenetic dysregulation in autism spectrum disorders. *Trends Mol Med.* 2024;30(11):1028-1046.
doi: 10.1016/j.molmed.2024.06.004
 401. Rittiner J, Cumarana M, Malhotra S, Kantor B. Therapeutic modulation of gene expression in the disease state: Treatment strategies and approaches for the development of next-generation of the epigenetic drugs. *Front Bioeng Biotechnol.* 2022;10:1035543.
doi: 10.3389/fbioe.2022.1035543
 402. Devos Y, Mumford JD, Bonsall MB, et al. Potential use of gene drive modified insects against disease vectors, agricultural pests and invasive species poses new challenges for risk assessment. *Crit Rev Biotechnol.* 2022;42:254-270.
doi: 10.1080/07388551.2021.1933891
 403. Jansson JK, McClure R, Egbert RG. Soil microbiome engineering for sustainability in a changing environment. *Nat Biotechnol.* 2023;41(12):1716-1728.
doi: 10.1038/s41587-023-01932-3
 404. Mamatha Bhanu LS, Katakai S, Chatterjee S. CRISPR: New promising biotechnological tool in wastewater treatment. *J Microbiol Methods.* 2024;227:107066.
doi: 10.1016/j.mimet.2024.107066
 405. Thakur N, Nigam M, Mann NA, et al. Host-mediated gene engineering and microbiome-based technology optimization for sustainable agriculture and environment. *Funct Integr Genomics.* 2023;23(1):57.
doi: 10.1007/s10142-023-00982-9
 406. Chen K, Shen Z, Wang G, et al. Research progress of CRISPR-based biosensors and bioassays for molecular diagnosis. *Front Bioeng Biotechnol.* 2022;10:986233.
doi: 10.3389/fbioe.2022.986233
 407. Wani AK, Akhtar N, Mir TG, et al. CRISPR/Cas12a-based biosensors for environmental monitoring and diagnostics. *Environ Technol Innov.* 2024;34:103625.
doi: 10.1016/j.eti.2024.103625
 408. Huang X, Yang D, Zhang J, Xu J, Chen YE. Recent advances in improving gene-editing specificity through CRISPR-Cas9 nuclease engineering. *Cells.* 2022;11(14):2186.
doi: 10.3390/cells11142186
 409. Ali N, Rampazzo RCP, Costa ADT, Krieger MA. Current nucleic acid extraction methods and their implications to point-of-care diagnostics. *Biomed Res Int.* 2017;2017:9306564.
doi: 10.1155/2017/9306564
 410. Liu CW, Tsutsui H. Sample-to-answer sensing technologies for nucleic acid preparation and detection in the field. *SLAS Technol.* 2023;28(5):302-323.
doi: 10.1016/j.slast.2023.06.002
 411. Hueso L, Martorell S, Sena-Torralba A, et al. Recombinase polymerase amplification technology for point-of-care diagnosis of neglected tropical diseases. *Int J Infect Dis.* 2025;153:107831.
doi: 10.1016/j.ijid.2025.107831
 412. Lee Y, Lee M, Shin Y, Kim K, Kim T. Spatial omics in clinical research: A comprehensive review of technologies and guidelines for applications. *Int J Mol Sci.* 2025;26(9):3949.
doi: 10.3390/ijms26093949
 413. Siddiqi S. The AJHCS strategic planning framework: Adapting government methodologies to enhance inpatient healthcare outcomes. *Am J Healthc Strategy.* 2024;1(2):1-5.
doi: 10.61449/ajhcs.2024.1
 414. Al-Akayleh F, Ali Agha ASA. Trust, ethics, and user-centric design in AI-integrated genomics. In: *2024 2nd International Conference on Cyber Resilience (ICCR).* 2024. p. 1-6.
doi: 10.1109/ICCR61006.2024.10532890
 415. Athanasopoulou K, Michalopoulou VI, Scorilas A, Adamopoulos PG. Integrating artificial intelligence in next-generation sequencing: Advances, challenges, and future directions. *Curr Issues Mol Biol.* 2025;47(6):470.
doi: 10.3390/cimb47060470
 416. Schlusser N, González A, Pandey M, Zavolan M. Current limitations in predicting mRNA translation with deep learning models. *Genome Biol.* 2024;25(1):227.
doi: 10.1186/s13059-024-03369-6
 417. *Lifecycle Governance for Explainable AI in Pharmaceutical Supply Chains: A Framework for Continuous Validation, Bias Auditing, and Equitable Healthcare Delivery.* Researchgate; 2025. Available from: <https://www.researchgate>.

- net/publication/390427090_lifecycle_governance_for_explainable_ai_in_pharmaceutical_supply_chains_a_framework_for_continuous_validation_bias_auditing_and_equitable_healthcare_delivery [Last accessed on 2025 Jul 07].
418. Kirpalani C, Kumar D. Integrating ethics and social responsibility in health informatics. In: Tripathi G, Shakya A, Kanga S, Guite LTS, Singh SK, editors. *Sustainability and Health Informatics: A Systems Approach to Address the Climate Action Induced Global Challenge*. Berlin: Springer Nature; 2024. p. 99-120. doi: 10.1007/978-981-97-6706-9_5
 419. Olaghere J, Williams DA, Farrar J, et al. Scientific advancements in gene therapies: Opportunities for global regulatory convergence. *Biomedicine*. 2025;13(3):758. doi: 10.3390/biomedicine13030758
 420. Ilcic A, Fuentes M, Lawler D. Artificial intelligence, complexity, and systemic resilience in global governance. *Front ArtifIntell*. 2025;8:1562095. doi: 10.3389/frai.2025.1562095
 421. Al-Ouqaili MTS, Ahmad A, Jwair NA, Al-Marzooq F. Harnessing bacterial immunity: CRISPR-Cas system as a versatile tool in combating pathogens and revolutionizing medicine. *Front Cell Infect Microbiol*. 2025;15:1588446. doi: 10.3389/fcimb.2025.1588446
 422. Ewaisha R, Anderson KS. Immunogenicity of CRISPR therapeutics-Critical considerations for clinical translation. *Front Bioeng Biotechnol*. 2023;11:1138596. doi: 10.3389/fbioe.2023.1138596
 423. Jia S, Lv H, Li Q, Fan C, Wang F. DNA-based biocomputing circuits and their biomedical applications. *Nat Rev Bioeng*. 2025;3:535-548. doi: 10.1038/s44222-025-00303-8
 424. Barrangou R, Fremaux C, Deveau H, et al. CRISPR provides acquired resistance against viruses in prokaryotes. *Science*. 2007;315(5819):1709-1712. doi: 10.1126/science.1138140
 425. Doudna JA, Charpentier E. The new frontier of genome engineering with CRISPR-Cas9. *Science*. 2014;346(6213):1258096. doi: 10.1126/science.1258096
 426. Mali P, Yang L, Esvelt KM, et al. RNA-guided human genome engineering via Cas9. *Science*. 2013;339(6121):823-826. doi: 10.1126/science.1232033
 427. Cong L, Ran FA, Cox D, et al. Multiplex genome engineering using CRISPR/Cas systems. *Science*. 2013;339(6121):819-823. doi: 10.1126/science.1231143
 428. Jinek M, Chylinski K, Fonfara I, Hauer M, Doudna JA, Charpentier E. A programmable dual-RNA-guided DNA endonuclease in adaptive bacterial immunity. *Science*. 2012;337(6096):816-821. doi: 10.1126/science.1225829
 429. Available from: <https://news.crisprtx.com/news-releases/news-release-details/crispr-therapeutics-and-vertex-establish-strategic-research> [Last accessed on 2025 Jul 16].
 430. *Editas Medicine, Inc. Common Stock (EDIT) Stock Price, Quote, News & History. Nasdaq*. Available from: <https://www.nasdaq.com/market-activity/stocks/edit> [Last accessed on 2025 Jul 16].
 431. *CRISPR Therapeutics AG Common Shares (CRSP) Stock Price, Quote, News & History. Nasdaq*. Available from: <https://www.nasdaq.com/market-activity/stocks/crsp> [Last accessed on 2025 Jul 16].
 432. *Intellia Therapeutics, Inc. Common Stock (NTLA) Stock Price, Quote, News & History. Nasdaq*. Available from: <https://www.nasdaq.com/market-activity/stocks/ntla> [Last accessed on 2025 Jul 16].
 433. Frangoul H, Altshuler D, Cappellini MD, et al. CRISPR-Cas9 gene editing for sickle cell disease and β -thalassemia. *N Engl J Med*. 2021;384(3):252-260. doi: 10.1056/NEJMoa2031054
 434. Vertex Pharmaceuticals Incorporated. *A Phase 1/2/3 Study of the Safety and Efficacy of a Single Dose of Autologous CRISPR-Cas9 Modified CD34+ Human Hematopoietic Stem and Progenitor Cells (hHSPCs) in Subjects With Transfusion-Dependent β -Thalassemia*; 2025. Available from: <https://clinicaltrials.gov/study/NCT03655678> [Last accessed on 2025 Jul 16].
 435. Celgene. *A Phase 3, Multicenter, Randomized, Open-Label Study to Compare the Efficacy and Safety of Bb2121 Versus Standard Regimens in Subjects With Relapsed and Refractory Multiple Myeloma (RRMM) (KarMMa-3)*; 2022. Available from: <https://clinicaltrials.gov/study/NCT03651128> [Last accessed on 2025 Jul 16].
 436. *The Nobel Prize in Chemistry 2020*. Available from: <https://www.nobelprize.org/prizes/chemistry/2020/summary> [Last accessed on 2025 Jul 16].
 437. STAT. Available from: <https://www.statnews.com> [Last accessed on 2025 Jul 16].
 438. *Commissioner O of the. News & Events. FDA*; 2024. Available from: <https://www.fda.gov/news-events> [Last accessed on 2025 Jul 16].
 439. *CRISPR-Based Gene Editing Market Size to Hit USD 13.39 Billion by 2034*. Available from: <https://www.precedenceresearch.com/crispr-based-gene-editing-market> [Last accessed on 2025 Jul 16].
 440. *Grand View Research*. Available from: <https://www.grandviewresearch.com/industry-analysis/crispr-genome-editing-market> [Last accessed on 2025 Jul 16].
 441. *Commissioner O of the. FDA Approves First Gene Therapies to Treat Patients with Sickle Cell Disease*. FDA. Available from: <https://www.fda.gov/news-events/press-announcements/fda-approves-first-gene-therapies-treat-patients-sickle-cell-disease> [Last accessed on 2025 May 22].
 442. *Editas Medicine Announces New EDIT-301 Safety and Efficacy Data in 17 Patients, Presented Today at the American Society of Hematology (ASH) Annual Meeting and in a Company-sponsored Webinar. Editas Medicine*. Available from: <https://ir.editasmedicine.com/news-releases/news-release-details/editas-medicine-announces-new-edit-301-safety-and-efficacy-data> [Last accessed on 2025 May 22].
 443. *Beam Therapeutics to Highlight New Data from BEAM-101 Program in Sickle Cell Disease at European Hematology Association (EHA) 2025 Congress. Beam Therapeutics*. Available from: <https://investors.beamtx.com/news-releases/news-release-details/beam-therapeutics-highlight-new-data-beam-101-program-sickle> [Last accessed on 2025 May 22].
 444. *Intellia Therapeutics Announces First Patient Dosed in the Phase 3 MAGNITUDE Study of NTLA-2001 as a Single-Dose CRISPR-Based Treatment for Transthyretin Amyloidosis with Cardiomyopathy - Intellia Therapeutics*. Available from: <https://ir.intelliatx.com/news-releases/news-release-details/intellia-therapeutics-announces-first-patient-dosed-phase-3> [Last accessed on 2025 May 22].
 445. Marrugo-Ramirez J, Mir M, Samitier J. Blood-based cancer biomarkers in liquid biopsy: A promising non-invasive alternative to tissue biopsy. *Int J Mol Sci*. 2018;19(10):2877. doi: 10.3390/ijms19102877
 446. Durán-Vinet B, Araya-Castro K, Calderón J, et al. CRISPR/Cas13-based platforms for a potential next-generation diagnosis of colorectal cancer through exosomes micro-RNA detection: A review. *Cancers*. 2021;13(18):4640. doi: 10.3390/cancers13184640
 447. Acharya D, Mukhopadhyay A. A comprehensive review of machine learning techniques for multi-omics data integration: Challenges and applications in precision oncology. *Brief Funct Genomics*. 2024;23(5):549-560. doi: 10.1093/bfpg/ela013
 448. Abbasi AF, Asim MN, Dengel A. Transitioning from wet lab to artificial intelligence: A systematic review of AI predictors in CRISPR. *J Transl Med*. 2025;23(1):153. doi: 10.1186/s12967-024-06013-w

Received: July 22, 2025

Revised: August 25, 2025

Accepted: August 28, 2025

Available online: October 28, 2025